



TEST REPORT

Product Name: hydrogen inhalation machine
Trade Mark: N/A
Model No.: OL-225
Add. Model No.: OL-300, OL-450, OL-600, OL-900, OL-1200,
OL-1500, OL-2000, OL-3000, OL-900D
Report Number: JAT250205044S2-ER00
Test Standards: EN IEC 55014-1:2021
EN IEC 55014-2:2021
EN IEC 61000-3-2:2019/A2:2024
EN 61000-3-3:2013/A2:2021
Directive: 2014/30/EU
Test Result: PASS
Date of Issue: 2025-02-14

Prepared for:

OLang Technology Co.,Ltd.
No.25 Dongpo street,Dongping Area Huizhou Guangdong China

Prepared by:

Dongguan Jun'an Testing & Certification Co., Ltd.
Room 303, Building 1, No.316, Renzhou Road, Shatian Town, Dongguan
City, Guangdong Province, China.



Prepared by: Tanac *Tanac*

Reviewed by: Roger ZHENG *Roger ZHENG*

Approved by: Tim You *Tim you*





Version

| Version No. | Date | Description |
|-------------|------------|-------------|
| 00 | 2025-02-14 | Original |
| | | |



CONTENTS

| | |
|--|-----------|
| 1. GENERAL INFORMATION..... | 5 |
| 1.1 CLIENT INFORMATION..... | 5 |
| 1.2 EUT INFORMATION..... | 5 |
| 1.2.1 GENERAL DESCRIPTION OF EUT..... | 5 |
| 1.2.2 DESCRIPTION OF ACCESSORIES..... | 5 |
| 1.3 DESCRIPTION OF SUPPORT UNITS..... | 5 |
| 1.4 TEST LOCATION..... | 6 |
| 1.5 TEST FACILITY..... | 6 |
| 1.6 DEVIATION FROM STANDARDS..... | 6 |
| 1.7 ABNORMALITIES FROM STANDARD CONDITIONS..... | 6 |
| 1.8 OTHER INFORMATION REQUESTED BY THE CUSTOMER..... | 6 |
| 1.9 MEASUREMENT UNCERTAINTY..... | 7 |
| 2. TEST SUMMARY..... | 8 |
| 3. EQUIPMENT LIST..... | 9 |
| 4. TEST CONFIGURATION..... | 11 |
| 4.1 ENVIRONMENTAL CONDITIONS FOR TESTING..... | 11 |
| 4.1.1 NORMAL OR EXTREME TEST CONDITIONS..... | 11 |
| 4.1.2 RECORD OF NORMAL ENVIRONMENT..... | 11 |
| 4.2 TEST MODES..... | 11 |
| 5. PERFORMANCE CRITERIA..... | 12 |
| 6. EMC REQUIREMENTS SPECIFICATION..... | 13 |
| 6.1 REFERENCE DOCUMENTS FOR TESTING..... | 13 |
| 6.2 EMISSION..... | 14 |
| 6.2.1 DISTURBANCE POWER..... | 15 |
| 6.2.2 MAINS/LOAD/CONTROL TERMINAL DISTURBANCE VOLTAGE (150 KHZ TO 30 MHZ)..... | 17 |
| 6.3 IMMUNITY..... | 21 |
| 6.3.1 ELECTROSTATIC DISCHARGE..... | 22 |
| 6.3.2 RADIO FREQUENCY ELECTROMAGNETIC FIELDS, 80 MHZ TO 1 000 MHZ..... | 25 |
| 6.3.3 FAST TRANSIENTS..... | 27 |
| 6.3.4 INJECTED CURRENTS..... | 30 |
| 6.3.5 SURGES..... | 32 |
| 6.3.6 VOLTAGE DIPS..... | 34 |
| APPENDIX 1 PHOTOGRAPHS OF TEST SETUP..... | 36 |
| APPENDIX 2 PHOTOGRAPHS OF EUT CONSTRUCTIONAL DETAILS..... | 39 |
| EUT EXTERNAL PHOTOS..... | 39 |
| EUT INTERNAL PHOTOS..... | 41 |



1. GENERAL INFORMATION

1.1 CLIENT INFORMATION

| | |
|---------------------------------|---|
| Applicant: | OLang Technology Co.,Ltd. |
| Address of Applicant: | No.25 Dongpo street,Dongping Area Huizhou Guangdong China |
| Manufacturer: | OLang Technology Co.,Ltd. |
| Address of Manufacturer: | No.25 Dongpo street,Dongping Area Huizhou Guangdong China |

1.2 EUT INFORMATION

1.2.1 General Description of EUT

| | |
|------------------------------|---|
| Product Name: | hydrogen inhalation machine |
| Model No.: | OL-225 |
| Add. Model No.: | OL-300, OL-450, OL-600, OL-900, OL-1200, OL-1500, OL-2000, OL-3000, OL-900D |
| Trade Mark: | N/A |
| DUT Stage: | Production Unit |
| Power Supply: | 110-240V~ 50/60Hz, 150W |
| Product Category: | All equipment |
| Sample Received Date: | 2025-02-05 |
| Sample Tested Date: | 2025-02-05~2025-02-11 |

1.2.2 Description of Accessories

None.

1.3 DESCRIPTION OF SUPPORT UNITS

None.



1.4 TEST LOCATION

Dongguan Jun'an Testing & Certification Co., Ltd.

Address: Room 303, Building 1, No.316, Renzhou Road, Shatian Town, Dongguan City, Guangdong Province, China.

1.5 TEST FACILITY

The test facility is recognized, certified, or accredited by the following organizations:

Dongguan Jun'an Testing & Certification Co., Ltd.

1.6 DEVIATION FROM STANDARDS

None.

1.7 ABNORMALITIES FROM STANDARD CONDITIONS

None.

1.8 OTHER INFORMATION REQUESTED BY THE CUSTOMER

None.



1.9 MEASUREMENT UNCERTAINTY

| No. | Item | Measurement Uncertainty |
|-----|--|-------------------------|
| 1 | Conducted emission 9kHz-150kHz (AMN) | ±3.2 dB |
| 2 | Conducted emission 150kHz-30MHz (AMN) | ±2.7 dB |
| 3 | Asymmetric mode conducted emissions (AAN) Network port (150kHz-30MHz) | ±2.1 dB |
| 4 | Conducted differential voltage emissions Antenna port (150kHz-30MHz) | ±1.6 dB |
| 5 | Asymmetric mode conducted emissions Signal, Tuner port (150kHz-30MHz) | ±2.1 dB |
| 6 | Radiated emission 30MHz-1GHz (SAC) | ± 4.6 dB |
| 7 | Radiated emission 1GHz-18GHz (FAR) | ± 4.4 dB |
| 8 | Harmonic current emissions | ±1.4% |
| 9 | Voltage fluctuations and flicker | ±1.4% |

Remark: 95% Confidence Levels, k=2.

2. TEST SUMMARY

| Part 1: Emission requirements | | | | |
|--|--|---------------------|------------|-------------------------------|
| Test Item | | EN IEC 55014-1:2021 | | Results |
| | | Test Requirement | Limits | |
| Continuous disturbances | Disturbance voltage (9 kHz to 30 MHz) | Clause 4.3.2 | Table 2 | NA ^(See Note 1, 2) |
| | Magnetic field strength (9 kHz to 30 MHz) | Clause 4.3.2 | Table 3 | NA ^(See Note 1, 2) |
| | Magnetic field induced current (9 kHz to 30 MHz) | Clause 4.3.2 | Table 4 | NA ^(See Note 1, 2) |
| | Disturbance voltage (150 kHz to 30 MHz) | Clause 4.3.3 | Table 5, 6 | PASS |
| | Disturbance power (30 MHz to 300 MHz) | Clause 4.3.4 | Table 7, 8 | NA ^(See Note 1, 3) |
| | Radiated disturbance (30 MHz to 1 000 MHz) | Clause 4.3.4 | Table 9 | PASS |
| Discontinuous disturbances | Clicks (150 kHz to 30 MHz) | Clause 4.4 | Clause 4.2 | NA ^(See Note 1, 4) |
| Note: 1) N/A: In the whole report not applicable. 2) It only apply to induction cooking appliances. 3) The Manufacturer choice Radiated emission Measurement 30MHz to 1000MHz. 4) This product does not have a switch operated controller and thermostat. | | | | |

| Part 2: Immunity requirements | | | |
|---|--|---|---------|
| Test Item | Test Requirement (EN IEC 55014-2:2021) | Test Method | Results |
| Electrostatic discharge | Clause 5.1 | IEC 61000-4-2:2008 | Pass |
| Fast transients | Clause 5.2 | IEC 61000-4-4:2012 | Pass |
| Injected currents | Clause 5.3, 5.4 | IEC 61000-4-6:2013 | Pass |
| Radio frequency electromagnetic fields, 80 MHz to 1 000 MHz | Clause 5.5 | IEC 61000-4-3:2006+A1:2007+A2:2010 IEC 61000-4-22:2010 | Pass |
| Surges | Clause 5.6 | IEC 61000-4-5:2014 | Pass |
| Voltage dips | Clause 5.7 | IEC 61000-4-11:2004 | Pass |



3. EQUIPMENT LIST

Dongguan Jun'an Testing & Certification Co., Ltd.

3.1 MEASUREMENT INSTRUMENTS LIST

| Item | Equipment | Manufacturer | Model No. | Serial No. | Calibration time | Recalibration time |
|------|---------------------------------|--------------|-------------------|------------|------------------|--------------------|
| 1. | Test Receiver | Rohde&Schwar | ESC17(9 kHz-7GHz) | 100336 | Nov.10.2024 | Nov.09,2025 |
| 2. | Broadband antenna | Schwarzbeck | VULB9168 | 01222 | Nov.07,2024 | Nov.06,2025 |
| 3. | Horn antenna | Schwarzbeck | BBHA9120D | 02476 | Nov.14,2024 | Nov.13,2025 |
| 4. | Preamplifier | Schwarzbeck | BBV9745 | 00250 | Nov.09,2024 | Nov.08,2025 |
| 5. | Preamplifier | N/A | TRLA-01018G440B | 21081001 | Nov.09.2024 | Nov.08.2025 |
| 6. | 3M method semi anechoic chamber | SKET | 9m*6m*6m | 2021082304 | Oct.14,2024 | Oct.13,2025 |
| 7. | Pointer hygrometer | M&G | ARC92570 | N/A | Oct.29.2024 | Oct.28.2025 |

3.2For Electrostatic Discharge Immunity Test

| Item | Equipment | Manufacturer | Model No. | Serial No. | Last Cal | Recalibration time |
|------|--------------------------------|--------------|-----------|------------|-------------|--------------------|
| 1. | Electrostatic analog generator | LIONCEL | ESD-203B | 0210502 | Nov.16,2024 | Nov.15,2025 |



4. TEST CONFIGURATION

4.1 ENVIRONMENTAL CONDITIONS FOR TESTING

4.1.1 Normal or Extreme Test Conditions

| Environment Parameter | Selected Values During Tests | | |
|---|------------------------------|--------------|--|
| Test Condition | Ambient | | |
| | Temperature (°C) | Voltage | Relative Humidity (%) |
| NT/NV | +15 to +35 | AC 230V/50Hz | 20 to 75 (Except Electrostatic Discharge is 30 to 60) |
| Remark: 1) NV: Normal Voltage; NT: Normal Temperature | | | |

4.1.2 Record of Normal Environment

| Test Item | Temperature (°C) | Relative Humidity (%) | Pressure (Kpa) | Tested by |
|--|------------------|-----------------------|----------------|-----------|
| Disturbance Power | 24.8 | 54.9 | 98.56 | Alan Li |
| Conducted Emission | 24.8 | 54.9 | 98.56 | Alan Li |
| Harmonic Current Emissions | 25.6 | 56.0 | 98.90 | Alan Li |
| Voltage Fluctuations and Flicker | 25.6 | 56.0 | 98.90 | Alan Li |
| Electrostatic Discharge | 27.0 | 43.0 | 98.90 | Alan Li |
| Radio frequency electromagnetic fields | 25.3 | 53.1 | 98.90 | Alan Li |
| Electrical fast transients/burst | 25.6 | 56.0 | 98.90 | Alan Li |
| Surges | 25.6 | 56.0 | 98.90 | Alan Li |
| Continuous induced RF disturbances | 25.6 | 56.0 | 98.90 | Alan Li |
| Voltage dips and Voltage interruptions | 25.6 | 56.0 | 98.90 | Alan Li |

4.2 TEST MODES

| Test Modes | |
|---|------------------|
| AC mains power ports | TM1: Normal work |
| Radiated disturbance (30 MHz to 1 000 MHz) | TM1: Normal work |
| Harmonic Current Emissions | TM1: Normal work |
| Voltage Fluctuations and Flicker | TM1: Normal work |
| Electrostatic discharge | TM1: Normal work |
| Radio frequency electromagnetic fields, 80 MHz to 1 000 MHz | TM1: Normal work |
| Electrical fast transients/burst | TM1: Normal work |
| Surges | TM1: Normal work |
| Continuous induced RF disturbances | TM1: Normal work |
| Voltage dips and Voltage interruptions | TM1: Normal work |



5. PERFORMANCE CRITERIA

A functional description and a definition of performance criteria, during or as a consequence of the EMC testing, shall be provided by the manufacturer and noted in the test report, based on the following criteria.

➤ **Performance criterion A:**

The apparatus shall continue to operate as intended during the test. No degradation of performance or loss of function is allowed below a performance level (or permissible loss of performance) specified by the manufacturer, when the apparatus is used as intended. If the minimum performance level or the permissible performance loss is not specified by the manufacturer, then either of these may be derived from the product

➤ **<Performance criterion B>**

The apparatus shall continue to operate as intended after the test. No degradation of performance or loss of function is allowed below a performance level (or permissible loss of performance) specified by the manufacturer, when the apparatus is used as intended. During the test, degradation of performance is allowed, however no change of actual operating state or stored data is allowed to persist after the test. If the minimum performance level or the permissible performance loss is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and from what the user may reasonably expect from the apparatus if used as intended.

➤ **<Performance criterion C>**

Temporary loss of function is allowed, provided the function is self recoverable or can be restored by the operation of the controls, or by any operation specified in the instructions for use.

The selection, the specification of functions, and the permissible degradation is left to the responsibility of the manufacturer.

Annex A serves as a guide to formulate the permissible degradation of the equipment under test (EUT) caused by electromagnetic phenomena.

6. EMC REQUIREMENTS SPECIFICATION

6.1 REFERENCE DOCUMENTS FOR TESTING

EN IEC 55014-1:2021

Electromagnetic compatibility — Requirements for household appliances, electric tools and similar apparatus
Part 1: Emission

EN IEC 55014-2:2021

Electromagnetic compatibility — Requirements for household appliances, electric tools and similar apparatus
Part 2: Immunity — Product family standard

EN IEC61000-3-2:2019/A2:2024

Electromagnetic compatibility (EMC) Part 3-2: Limits — Limits for harmonic current emissions (equipment input current ≤ 16 A per phase)

EN 61000-3-3:2013/A2:2021

Electromagnetic compatibility (EMC) Part 3-3: Limits – Limitation of voltage changes, voltage fluctuations and flicker in public low-voltage supply systems, for equipment with rated current ≤ 16 A per phase and not subject to conditional connection

IEC 61000-4-2:2008

Electromagnetic compatibility (EMC) - Part 4-2: Testing and measurement techniques - Electrostatic discharge immunity test

IEC 61000-4-3:2006+A1:2007+A2:2010

Electromagnetic compatibility (EMC) - Part 4-3: Testing and measurement techniques - Radiated, radio-frequency, electromagnetic field immunity test

IEC 61000-4-4:2012

Electromagnetic compatibility (EMC) - Part 4-4: Testing and measurement techniques - Electrical fast transient/burst immunity test

IEC 61000-4-5:2005

Electromagnetic compatibility (EMC) - Part 4-5: Testing and measurement techniques - Surge immunity test

IEC 61000-4-6:2008

Electromagnetic compatibility (EMC) - Part 4-6: Testing and measurement techniques - Immunity to conducted disturbances, induced by radio-frequency fields

IEC 61000-4-8:2009

Electromagnetic compatibility (EMC) - Part 4-8: Testing and measurement techniques - Power frequency magnetic field immunity test

IEC 61000-4-11:2004

Electromagnetic compatibility (EMC) - Part 4-11: Testing and measurement techniques - Voltage dips, short interruptions and voltage variations immunity tests

IEC 61000-4-22:2010

Electromagnetic compatibility (EMC) – Part 4-22: Testing and measurement techniques - Radiated emission and immunity measurements in fully anechoic rooms (FARs)

6.2 EMISSION

Table 1 – Application of limits

| | | Disturbance voltage/ current | | | Disturbance voltage | Disturbance Power ^c | Radiated dist. | Magnetic field | | |
|-------------------------------------|--|------------------------------|---------|---------|---------------------|--------------------------------|----------------|----------------|---------|---------|
| | | Continuous ^{a, f} | | | Clicks ^b | | | (4.3.2) | | |
| Used | Sub clause | (4.3.2) | (4.3.3) | | (4.4.2) | (4.3.4) | | (4.3.4) | (4.3.2) | |
| | Limits | Table 2 | Table 5 | Table 2 | Text | Table 7 | Table 8 | Table 9 | Table 3 | Table 4 |
| <input checked="" type="checkbox"/> | All equipment not listed below | | • | | • | • | • | • | | |
| <input type="checkbox"/> | Tools | | | • | • | • | • | • | | |
| <input type="checkbox"/> | Induction cooking appliances | • | | | • | • | • | • | • | • |
| <input type="checkbox"/> | Electric fence energisers ^d | | • | | • | • | • | • | | |
| <input type="checkbox"/> | Toys Cat. A ^e | | | | | | | | | |
| <input type="checkbox"/> | Toys Cat. B | | | | | | | • | | |
| <input type="checkbox"/> | Toys Cat. C | | | | | | | • | | |
| <input type="checkbox"/> | Toys Cat. D | | • | | • | • | • | • | | |
| <input type="checkbox"/> | Toys Cat. E | | • | | • | • | • | • | | |

a. Limits of Table 5 and Table 6 can also be applicable to discontinuous disturbances (see 4.4.2.2).
b. For exemption and exceptions see 5.4.3.
c. For mains operated equipment, if certain conditions are met, the disturbance power test may be applied in alternative to the radiated disturbance test (see 4.3.4.2 and Figure 4).
d. For electric fence energisers the disturbance voltage test is applied according to 4.3.3.5.
e. Toys of category A shall be deemed to comply with the requirements of this standard without testing.
f. For wired network ports, see 4.3.3.7.

6.2.1 Disturbance power

Test Requirement: EN IEC 55014-1:2021 Clause 4.3.4

Receiver Setup:

| Frequency: (f) (MHz) | Detector type | Measurement receiver bandwidth | |
|-------------------------|---------------|--------------------------------|---------|
| | | RBW | VBW |
| 30 ≤ f ≤ 1 000 | Quasi Peak | 120 kHz | 300 kHz |

Measured frequency range

Limit:

| | General | | P ≤ 700 W | | 700 W < P ≤ 1 000 W | | P > 1 000 W | |
|-----------------------|--|----------|--|----------|--|----------|--|----------|
| Frequency range (MHz) | Limits dB(μW) Quasi-peak Average | | Limits dB(μW) Quasi-peak Average | | Limits dB(μW) Quasi-peak Average | | Limits dB(μW) Quasi-peak Average | |
| 30 ~ 300 | 45 ~ 55* | 35 ~ 45* | 45 ~ 55* | 35 ~ 45* | 30 ~ 300 | 45 ~ 55* | 35 ~ 45* | 45 ~ 55* |

Notes:

- * means the limit decreasing linearly with the logarithm of the frequency in the range 30MHz to 300MHz.
- If the quasi-peak measurements meet the average limit, the EUT shall be deemed to meet both limits and the measurements using the average detector need not be carried out.

Test Setup:

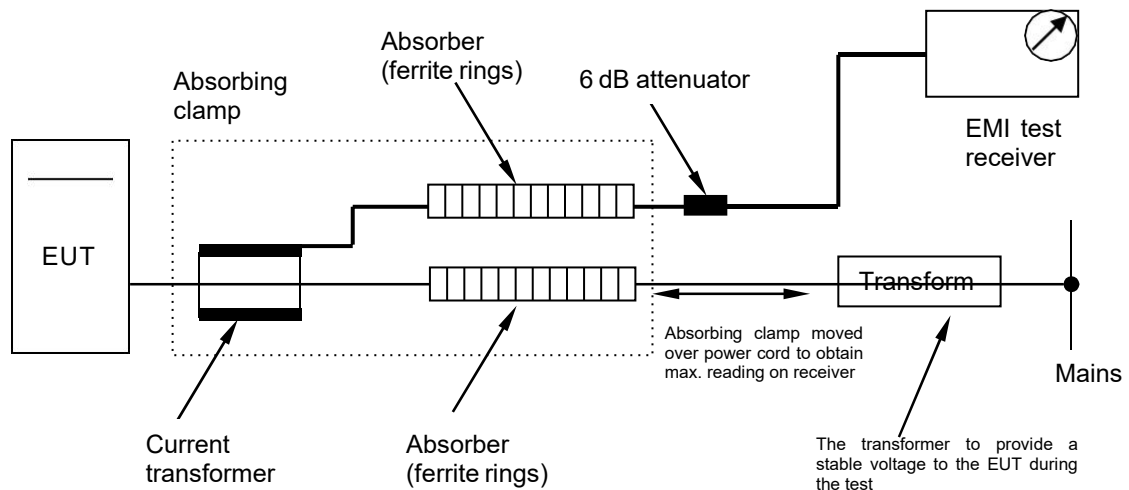


Figure 1. 6.2.1 Disturbance power

Test Procedures:


- 1) Measurement was performed in shielded room, and instruments used were according to clause 5.1 of EN 55014-1 if applicable.
- 2) Detailed test procedure and arrangement was according to clause 5.3 of EN 55014-1.
- 3) Measurement methods was according to clause 5.4 of EN 55014-1.
- 4) Operation conditions of EUT was according to clause 6 of EN 55014-1.
- 5) Frequency range 30MHz – 300MHz was checked and EMI receiver measurement bandwidth was set to 120kHz.


Equipment Used: Refer to section 3 for details.

Test Result: Pass



The measurement data as follows:

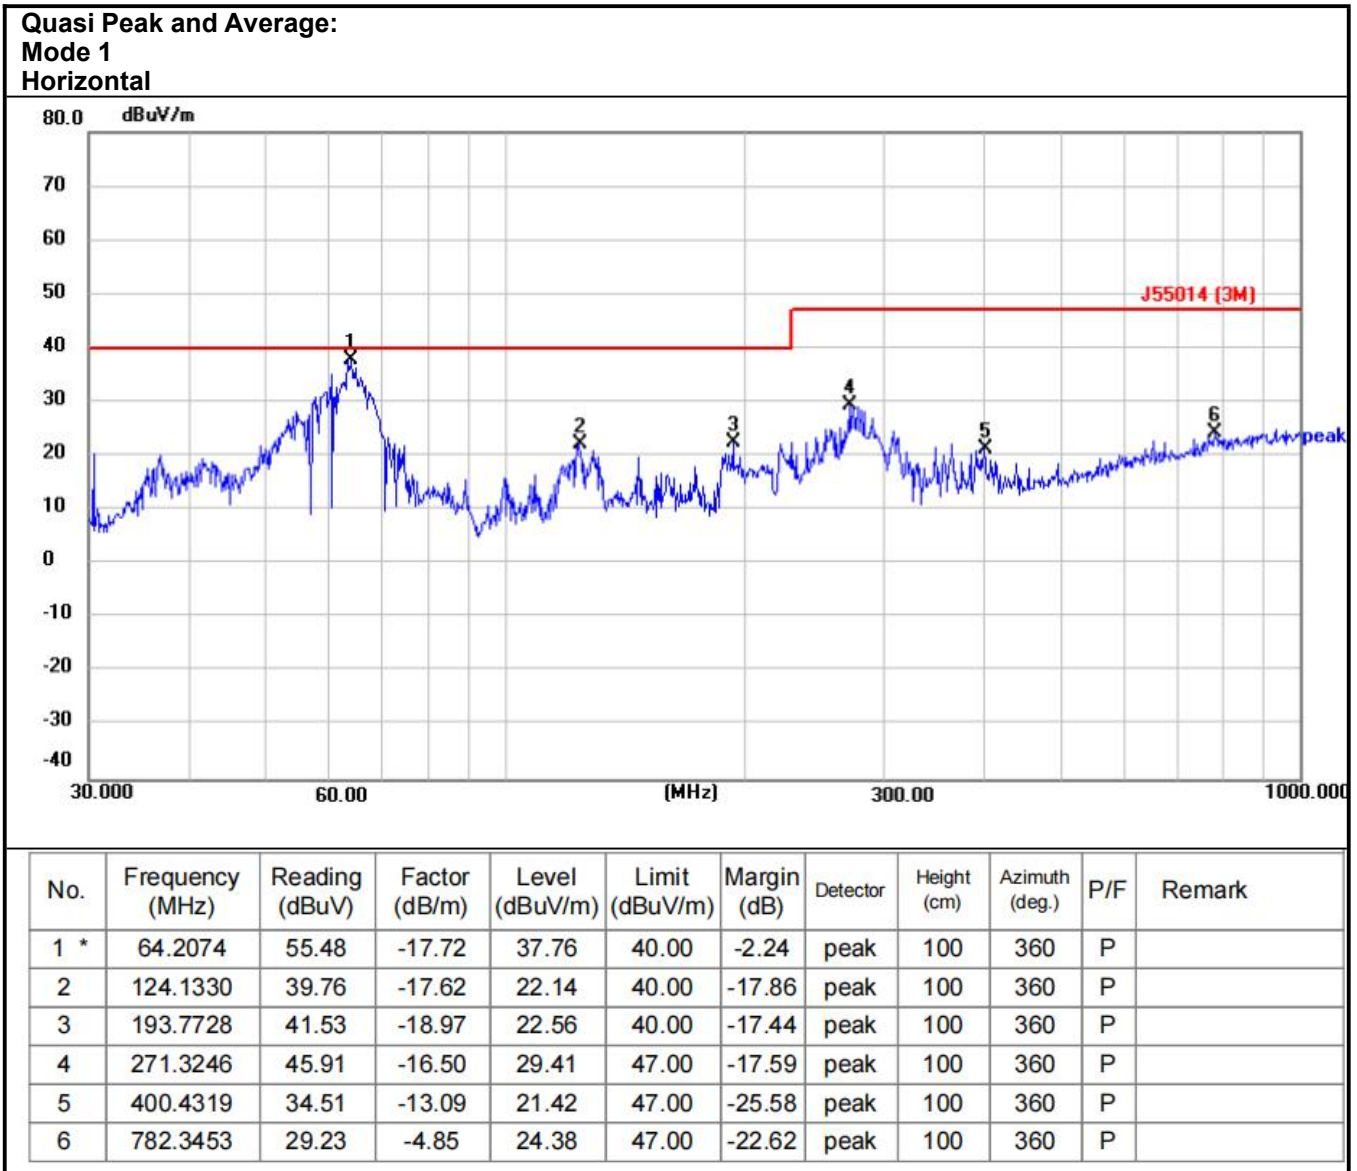

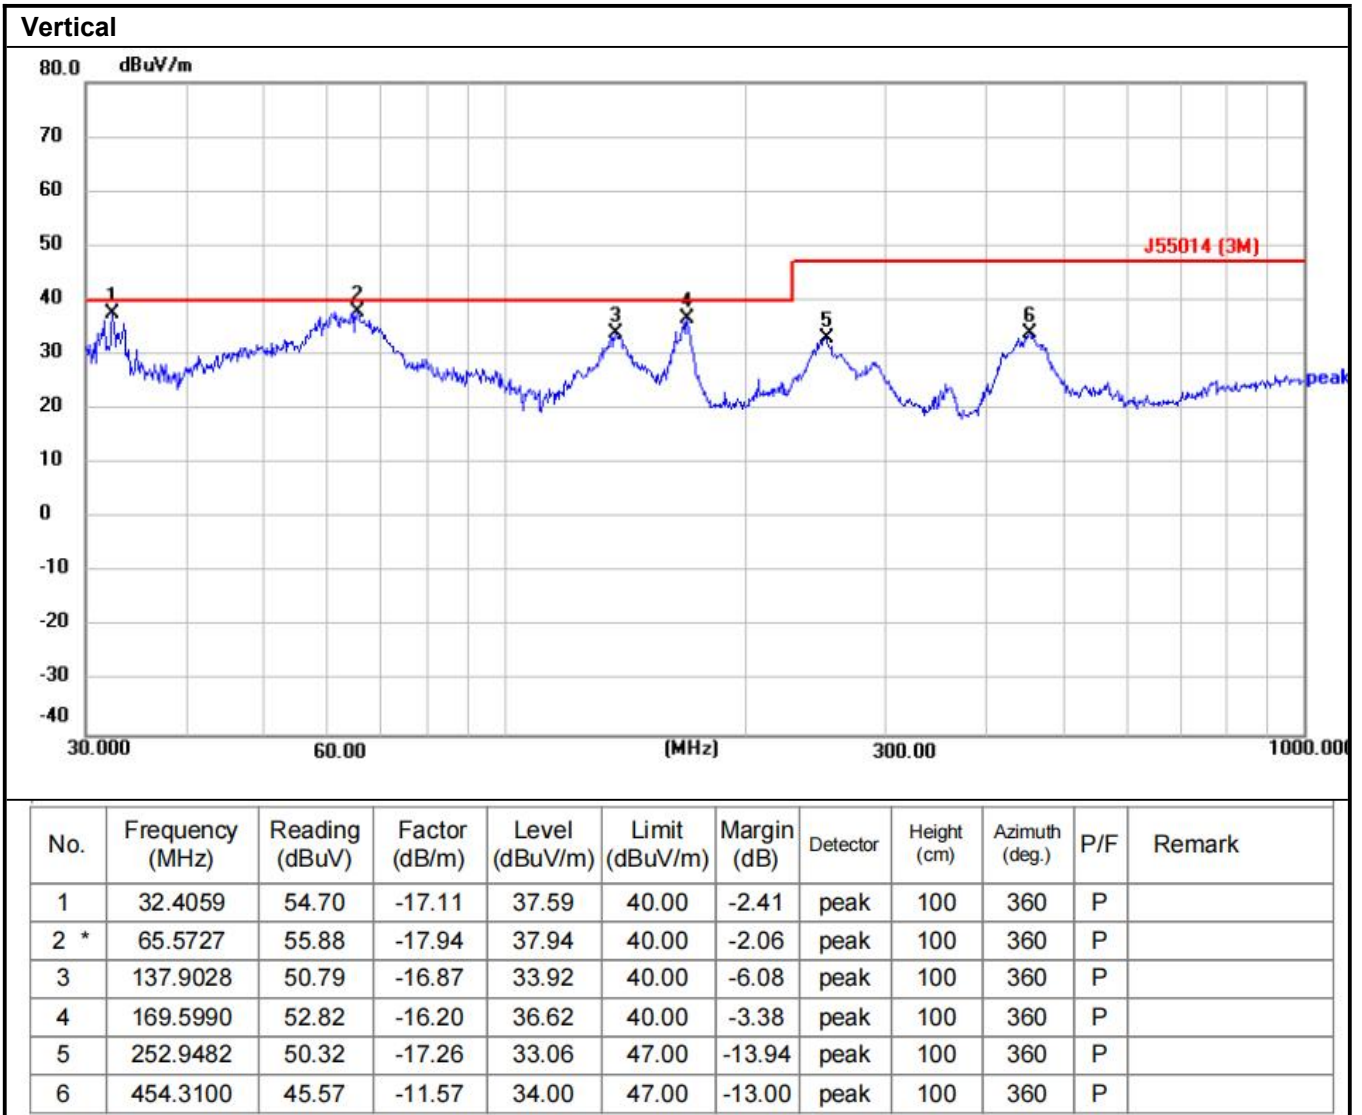

Remark:

1. Correct Factor = LISN Factor + Cable Loss + Pulse Limiter Factor, the value was added to Original Receiver Reading by the software automatically.
2. Result = Reading + Correct Factor.
3. Margin = Result - Limit

6.2.2 Mains/Load/Control Terminal Disturbance voltage (150 kHz to 30 MHz)

Test Requirement: EN IEC 55014-1:2021 Clause 4.3.2

Limit:

General limits

| Frequency range (MHz) | Mains ports | | Associated ports | | | |
|-----------------------|---------------------|-----------|---------------------|---------|---------------------|-----------|
| | Disturbance voltage | | Disturbance voltage | | Disturbance current | |
| | Limits dB(μV) | | Limits dB(μV) | | Limits dB(μV) | |
| | Quasi-peak | Average | Quasi-peak | Average | Quasi-peak | Average |
| 0.15 ~ 0.5 | 66 ~ 56 * | 66 ~ 56 * | 80 | 70 | 40 ~ 30 * | 30 ~ 20 * |
| 0.5 ~ 5.0 | 56 | 56 | 74 | 64 | 30 | 20 |
| 5.0 ~ 30 | 60 | 60 | 74 | 64 | | |

Notes:

- * means the limit decreasing linearly with the logarithm of the frequency in the range 0.15MHz to 0.5MHz.
- If the quasi-peak measurements meet the average limit, the EUT shall be deemed to meet both limits and the measurements using the average detector need not be carried out.


Limits for mains port of tools

| Frequency range (MHz) | P ≤ 700 W | | 700 W < P ≤ 1 000 W | | P > 1 000 W | |
|-----------------------|---------------|---------|---------------------|---------|---------------|-----------|
| | Limits dB(μV) | | Limits dB(μV) | | Limits dB(μV) | |
| | Quasi-peak | Average | Quasi-peak | Av rage | Quasi-peak | Average |
| 0.15-0.35 | 66-59* | 59-49* | 70-63* | 63-53* | 76 69* | 69 ~ 59 * |
| 0.35-5 | 59 | 49 | 63 | 53 | 69 | 59 |
| 5 30 | 64 | 54 | 68 | 58 | 74 | 64 |

Notes:


- * means the limit decreasing linearly with the logarithm of the frequency in the range 0.15MHz to 0.35MHz.
- If the quasi-peak measurements meet the average limit, the EUT shall be deemed to meet both limits and the measurements using the average detector need not be carried out.

Test Setup:

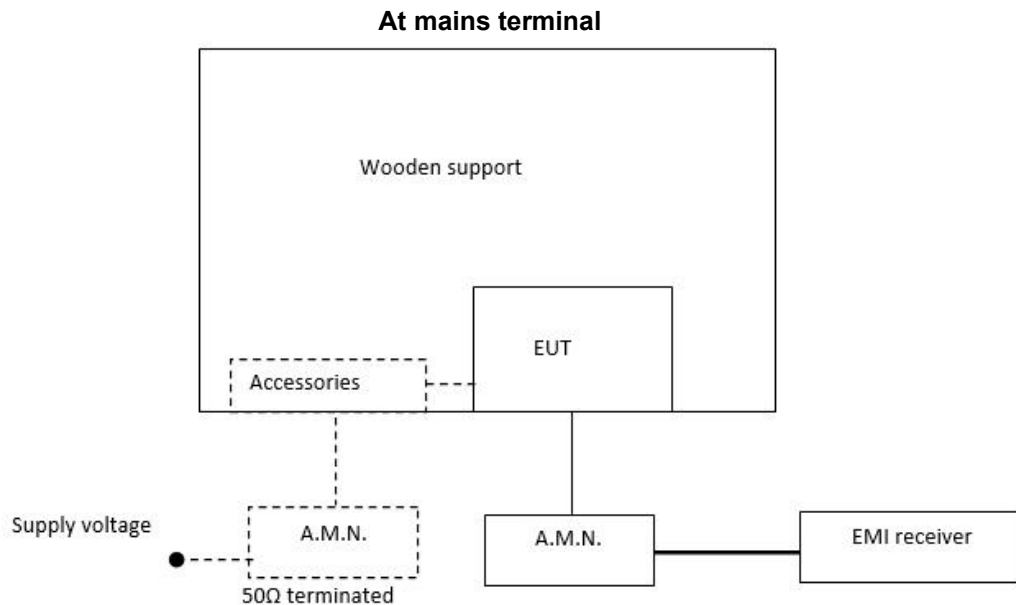

For table top equipment, wooden support is 0.8m height table

At Associated ports

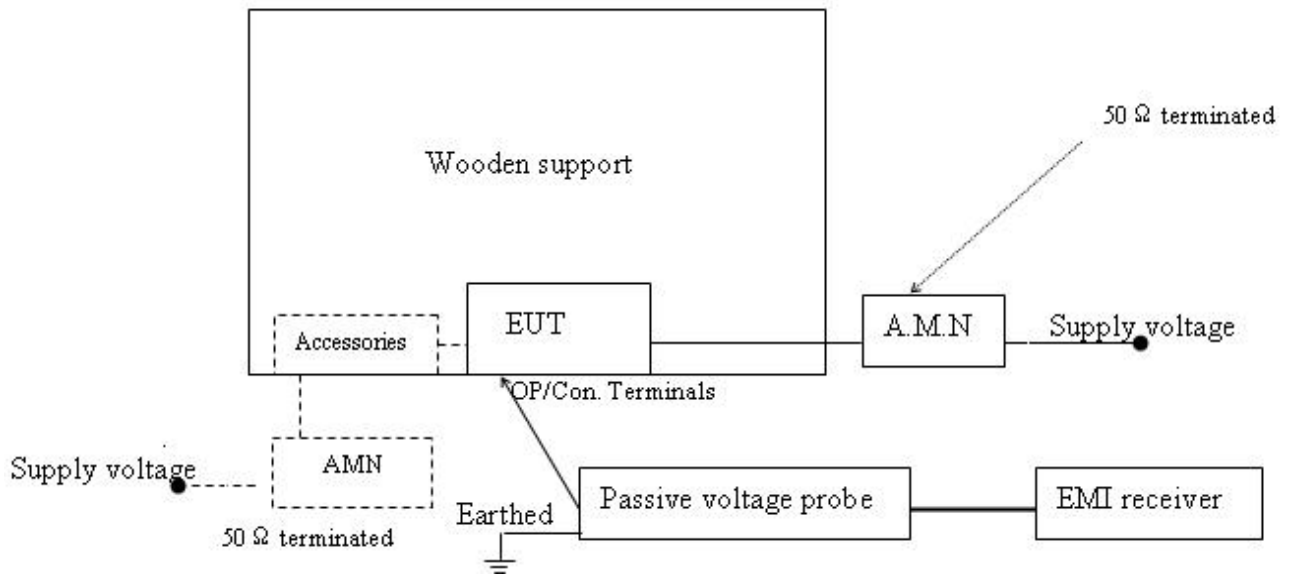

Note: : power line
 : signal line
 : means the test setup while available

Test Procedures: Detailed test procedure and arrangement was according to clause 5.2 of EN 55014-1.

- 1) The mains terminal disturbance voltage test was conducted in a shielded room.
- 2) The EUT was connected to AC power source through a LISN 1 (Line Impedance Stabilization Network) which provides a $50\Omega/50\mu\text{H} + 5\Omega$ linear impedance. The power cables of all other units of the EUT were connected to a second LISN 2, which was bonded to the ground reference plane in the same way as the LISN 1 for the unit being measured. A multiple socket outlet strip was used to connect multiple power cables to a single LISN provided the rating of the LISN was not exceeded.
- 3) The table top EUT was placed upon a non-metallic table 0.8 m above the ground reference plane. And for floor-standing arrangement, the EUT was placed on the horizontal ground reference plane.
- 4) The test was performed with a vertical ground reference plane. The rear of the EUT shall be 0.4 m from the vertical ground reference plane. The vertical ground reference plane was bonded to the horizontal ground reference plane. The LISN 1 was placed 0.8 m or 0.1 m from the boundary of the unit under test and bonded to a ground reference plane for LISNs mounted on top of the ground reference plane. This distance was between the closest points of the LISN 1 and the EUT. All other units of the EUT and associated equipment was at least 0.8 m from the LISN 2.

Equipment Used: Refer to section 3 for details.

Test Result: Pass



The measurement data as follows:

| |
|---|
| Quasi Peak and Average: Mode 1 |
| Live Line |
| N/A |



| Neutral Line |
|--------------|
| N/A |

Remark:


4. Correct Factor = LISN Factor + Cable Loss + Pulse Limiter Factor, the value was added to Original Receiver Reading by the software automatically.
5. Result = Reading + Correct Factor.
6. Margin = Result - Limit

6.2.3 Harmonic Current Emissions

Test Requirement: EN IEC 61000-3-2:2019/A2:2024 Clause 6.2.3

Test Method: The appropriate requirements of EN 61000-3-2/A1 for harmonic current emission apply for equipment covered by the scope of the present document with an input current up to and including 16A per phase. For equipment with an input current of greater than 16A per phase EN 61000-3-12 applies.

Test Setup:

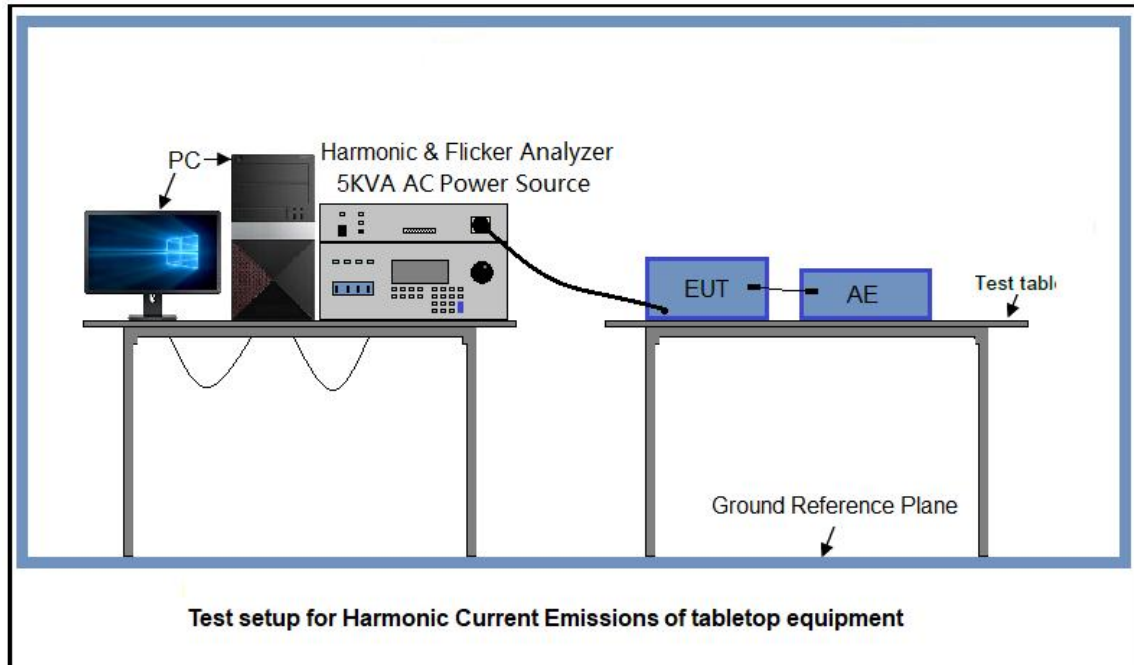

Equipment Used: Refer to section 3 for details.

Test Procedure: Harmonics of the fundamental current were measured up to 40 order harmonics using a digital power meter with an analogue output and frequency analyser which was integrated in the harmonic & flicker test system. The measurements were carried out under steady conditions.


6.2.4 Voltage Fluctuations and Flicker

Test Requirement: EN 61000-3-3:2013/A2:2021 Clause 4

Test Method: The appropriate requirements of EN 61000-3-3 for voltage fluctuations and flicker apply for equipment covered by the scope of the present document with an input current up to and including 16A per phase, if no conditional connection is needed. Where a conditional connection is required then the requirements of EN 61000-3-11 [12] shall apply.

For equipment with an input current of greater than 16A up to and including 75A per phase EN 61000-3-11 applies.

Test Setup:

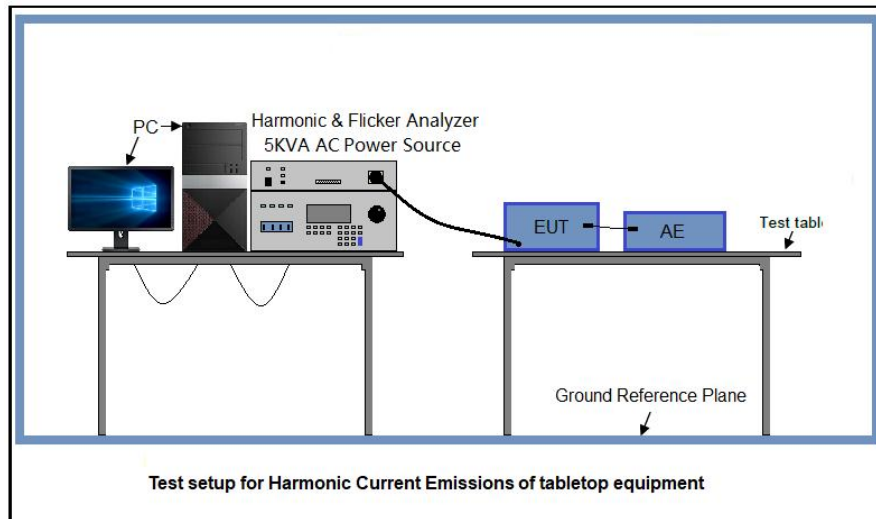


Equipment Used: Refer to section 3 for details.

Test Result: Pass

The measurement data as follows:

Flicker Test Summary per EN/IEC61000-3-3 Ed. 3.0 (2013) (Run time)

| | Result | Test Limit |
|----------------------|--------|------------|
| dt > 3.3 % (ms) | 0 | 500.0 |
| dc (%) | 0 | 3.30 |
| dmax (%) | 0.72 | 4.00 |
| Pst (10 min. period) | 0.28 | 1.000 |
| Pit (2 hr. period) | N/A | 0.650 |

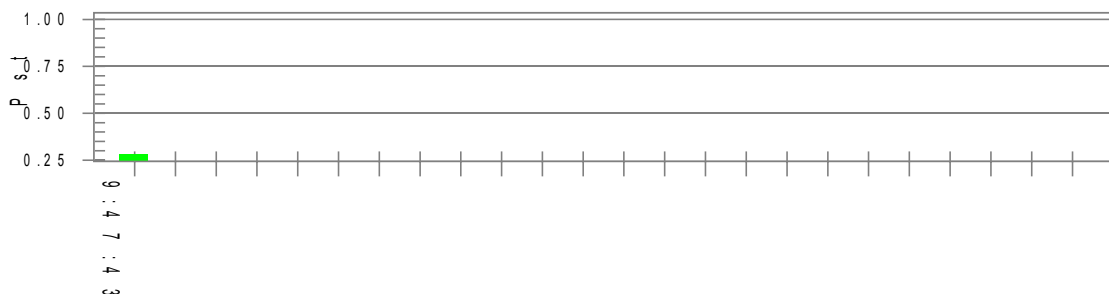



6.3 IMMUNITY


| Categories of apparatus | |
|---|--|
| <input type="checkbox"/> | Category I (fulfill the relevant immunity requirements without testing) |
| <input type="checkbox"/> | Category II (Shall fulfill the tests: ESD, EFT, Inject current, Surge, Dips) |
| <input type="checkbox"/> | Category III (Shall fulfill the tests: ESD, Radio frequency electromagnetic fields *) |
| <input checked="" type="checkbox"/> | Category IV (Shall fulfill the tests: ESD, EFT, Inject current, Surge, Dips, Radio frequency electromagnetic fields) |
| Note: *only applicable to the ride on toys operating with electronic devices. | |

6.3.1 Electrostatic Discharge

| | |
|-----------------------------|--|
| Test Requirement: | EN IEC 55014-2:2021 Clause 5.1 |
| Test Method: | The test method shall be in accordance with IEC 61000-4-2 |
| Criterion Required: | performance criteria B |
| Discharge Impedance: | 330 Ω / 150 pF |
| Polarity: | Positive & Negative |
| Number of Discharge: | Minimum 10 times at each test point |
| Discharge Mode: | Single Discharge |
| Discharge Period: | 1 second minimum |
| Test Level: | Contact discharge: Level 2, ± 4 kV Air discharge: Level 3, ± 8 kV |

Test Setup:


Test set-up for table-top equipment

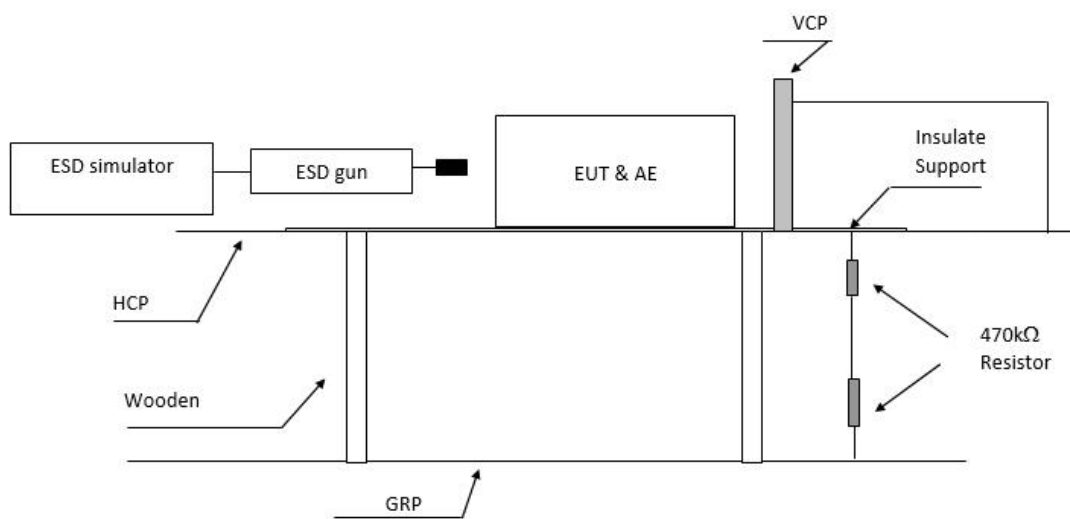

Note:

HCP means Horizontal Coupling Plane;
VCP means Vertical Coupling Plane;
GRP means Ground Reference Plane;
Wooden support is a 0.8m height table

Test setup for floor-standing equipment

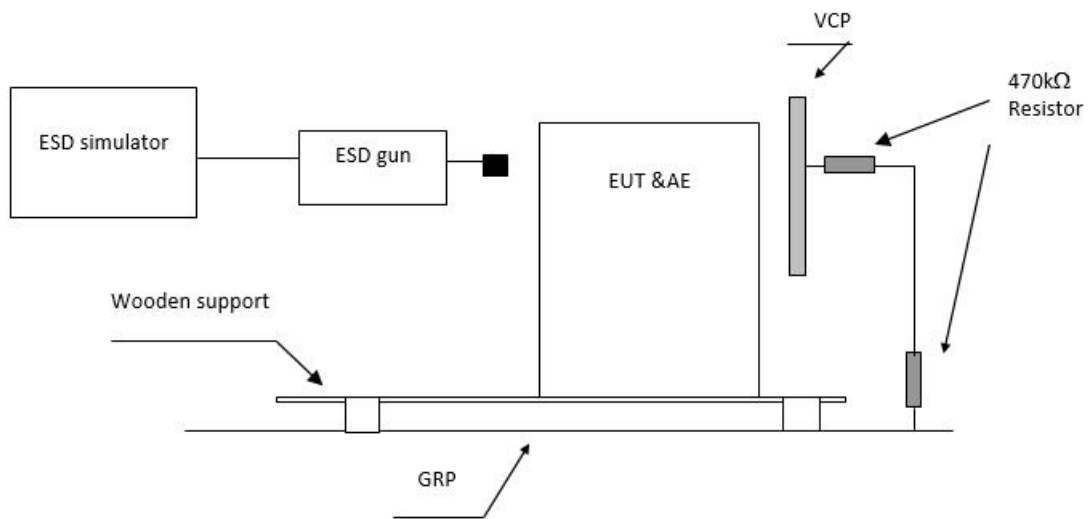

Note:

VCP means Vertical Coupling Plane;

GRP means Ground Reference Plane;

Wooden support is a 0.1m height rack

Test Procedures:

- 1) Electrostatic discharges shall be applied only to points and surfaces of the EUT which are expected to be touched during normal operation, including user access operations specified in the user manual, for example cleaning or adding consumables when the EUT is powered. The application of discharges to the contacts of open connectors is not required.
When applying direct discharges to a portable or handheld battery- powered EUT with a display screen, it may not be possible to observe the screen for a given EUT orientation. If observation of the screen is necessary during this test, the EUT may be mounted vertically using non - metallic supports.
- 2) The EUT was put on a 0.8m high wooden table for table-top equipment or 0.1m high for floor standing equipment standing on the ground reference plane (GRP).
- 3) A horizontal coupling plane(HCP) 1.6m by 0.8m in size was placed on the table, and the EUT with its cables were isolated from the HCP by an insulating support thick than 0.5mm. The VCP 0.5m by 0.5m in size & HCP were constructed from the same material type & think mess as that of the GRP, and connected to the GRP via a 470kΩ resistor at each end. The distance between EUT and any of the other metallic surface excepted the GRP, HCP and VCP was greater than 1m.
- 4) During the contact discharges, the tip of the discharge electrode was touch the EUT before the discharge switch is operated. During the air discharges, the round discharge tip of the discharge electrode was approached as fast as possible to touch the EUT.
- 5) After each discharge, the ESD generator was removed from the EUT, the generator was then retriggered for a new single discharge. For ungrounded product, a discharge cable with two resistances was used after each discharge to remove remnant electrostatic voltage. 10 times of each polarity single discharge were applied to HCP and VCP.

Equipment Used: Refer to section 3 for details.



Test Result: See below table.

| Discharge Type | Applied Voltage | Pulse No. | Result (Pursuant to EN IEC 55014-2:2021 Criterion B) | | |
|--|------------------------------------|--------------------|---|--|------------------------------|
| | | | <input checked="" type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input type="checkbox"/> N/A |
| Contact Discharge | ± 2 kV, ± 4 kV | 10 for every level | <input checked="" type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input type="checkbox"/> N/A |
| Air Discharge | ± 2 kV, ± 4 kV, ± 8 kV | 10 for every level | <input checked="" type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input type="checkbox"/> N/A |
| Indirect HCP Discharge | ± 4 kV | 10 for every level | <input checked="" type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input type="checkbox"/> N/A |
| Indirect VCP Discharge | ± 4 kV | 10 for every level | <input checked="" type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input type="checkbox"/> N/A |
| Remark: N/A: Not applicable | | | | | |
| Observation: <input checked="" type="checkbox"/> No observable change. <input type="checkbox"/> During the experiment, the following phenomena occurred: <hr/> | | | | | |
| Conclusion: The EUT met the requirements of the standard. | | | | | |

6.3.2 Radio frequency electromagnetic fields, 80 MHz to 1 000 MHz

- Test Requirement:** EN IEC 55014-2:2021 Clause 5.5
- Test Method:** The test method shall be in accordance with IEC 61000-4-3
- Criterion Required:** performance criteria A
- Frequency range:** 80 MHz to 1 000 MHz
- Test Level:** Level 2: 3 V/m(measured unmodulated)
- Modulation:** 1 kHz Sine wave, 80 % Amp. Modulation, audio signal of 400 Hz
- Frequency Step:** 1 % increment
- Dwell time:** 1 seconds
- Polarity Antenna:** Horizontal and vertical
- Test Setup:**

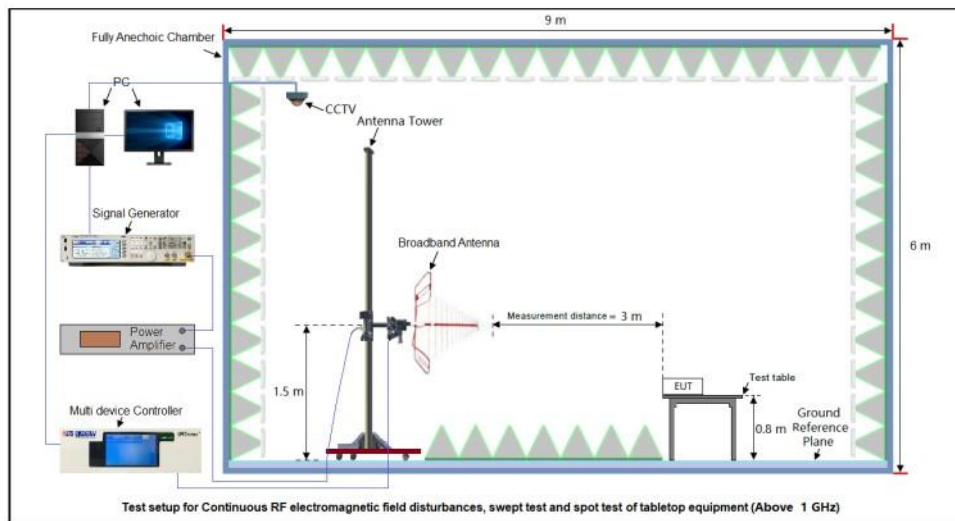


Figure 1. 80 MHz to 1 GHz

Test Procedures:

- 1) For table-top equipment, the EUT was placed in the chamber on a non-conductive table 0.8m high. For arrangement of floor-standing equipment, the EUT was mounted on a non-conductive support 0.1m above the supporting plane. For human body-mounted equipment, the EUT may be tested in the same manner as table top items.
- 2) If possible, a minimum of 1 m of cable is exposed to the electromagnetic field. Excess length of cables interconnecting units of the EUT shall be bundled low-inductively in the approximate center of the cable to form a bundle 30 cm to 40 cm in length.
- 3) The EUT was initially placed with one face coincident with the calibration plane. The EUT face being illuminated was contained within the UFA (Uniform Field Area).
- 4) The frequency ranges to be considered were swept with the signal modulated and pausing to adjust the RF signal level or to switch oscillators and antennas as necessary. Where the frequency range was swept incrementally, the step size was not exceed 10 % of the preceding frequency value.
- 5) The dwell time of the amplitude modulated carrier at each frequency was not be less than the time necessary for the EUT to be exercised and to respond, and was not less than 0.5 s.
- 6) The test normally was performed with the generating antenna facing each side of the EUT.
- 7) The polarization of the field generated by each antenna necessitates testing each selected side twice, once with the antenna positioned vertically and again with the antenna positioned horizontally.
- 8) The EUT was performed in a configuration to actual installation conditions, a video camera and/or an audio monitor were used to monitor the performance of the EUT.

Equipment Used: Refer to section 3 for details.



Test Result: See below table.

| EUT Face | Frequency | Level | Result (Pursuant to EN 55035 Criterion A) |
|--|------------------------------------|-------|--|
| Front | Swept test: 80 MHz to 1 000 MHz | 3 V/m | A |
| Back | | | A |
| Left | | | A |
| Right | | | A |
| Top | | | A |
| Under | | | A |
| Observation: <input checked="" type="checkbox"/> No observable change. <input type="checkbox"/> During the experiment, the following phenomena occurred: <hr/> | | | |
| Conclusion: The EUT met the requirements of the standard. | | | |

6.3.3 Fast transients

Test Requirement: EN IEC 55014-2:2021 Clause 5.2
Test Method: The test method shall be in accordance with EN 61000-4-4
Criterion Required: performance criteria B
Polarity: Positive & Negative


Test Level and Repetition Frequency:

| Open circuit output test voltage ($\pm 10\%$) and repetition rate of the impulses ($\pm 20\%$) | | | | |
|--|-----------------------------------|------------------------|---|------------------------|
| Level | Input and output a.c. power ports | | Input and output d.c. power ports Signal lines and control lines ports | |
| | Voltage peak kV | Repetition rate kHz | Voltage peak kV | Repetition rate kHz |
| 1 | 0.5 | 5 | 0.25 | 5 |
| 2 | 1 | 5 | 0.5 | 5 |
| 3 | 2 | 5 | 1 | 5 |
| 4 | 4 | 5 | 2 | 5 |
| X | Special | Special | Special | Special |


Notes :
 1. -XII is an open level. The level has to be specified in the dedicated equipment specification.
 2. The gray rows were the selected test level.

Impulse Wave shape: 5/50 ns
Burst Duration: 15ms
Burst Period: 300ms
Test Duration: 2 minute per level & polarity
Test Setup:

Test set-up for table-top equipment

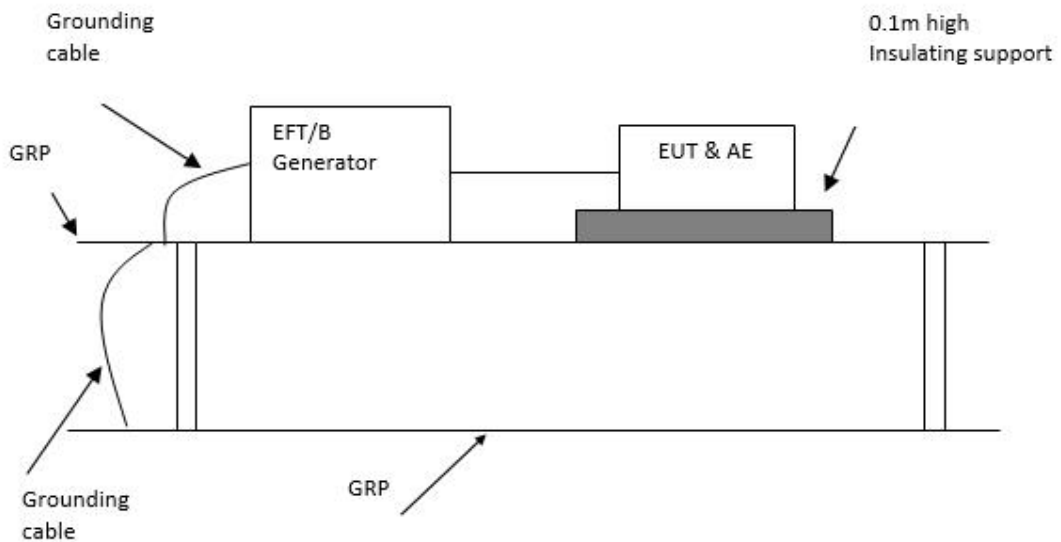


(for input a.c./d.c. power line)

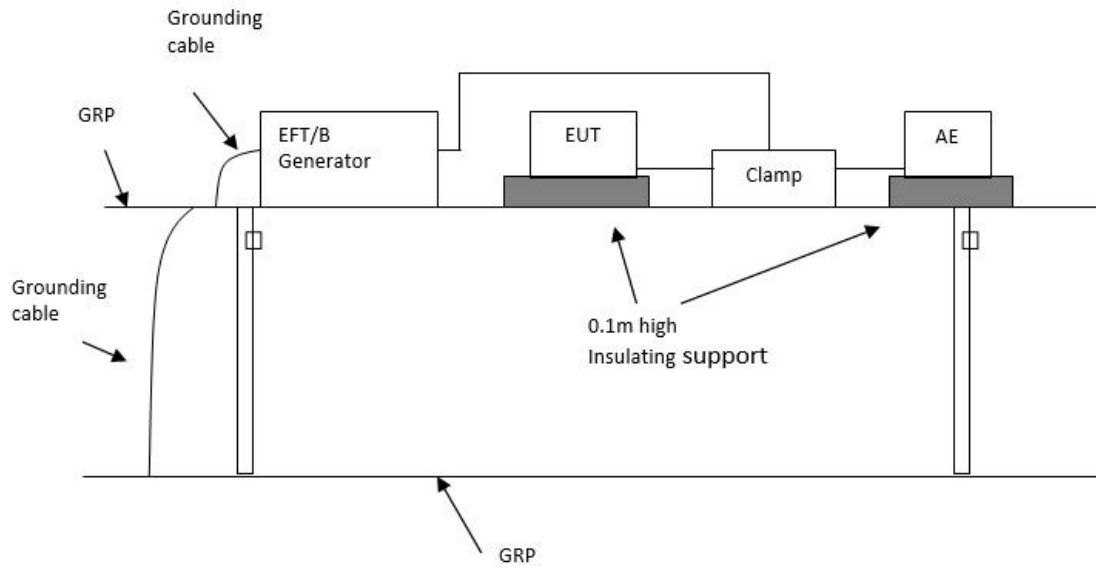


(for output a.c./d.c. power line or signal/control lines)

Test setup for floor-standing equipment

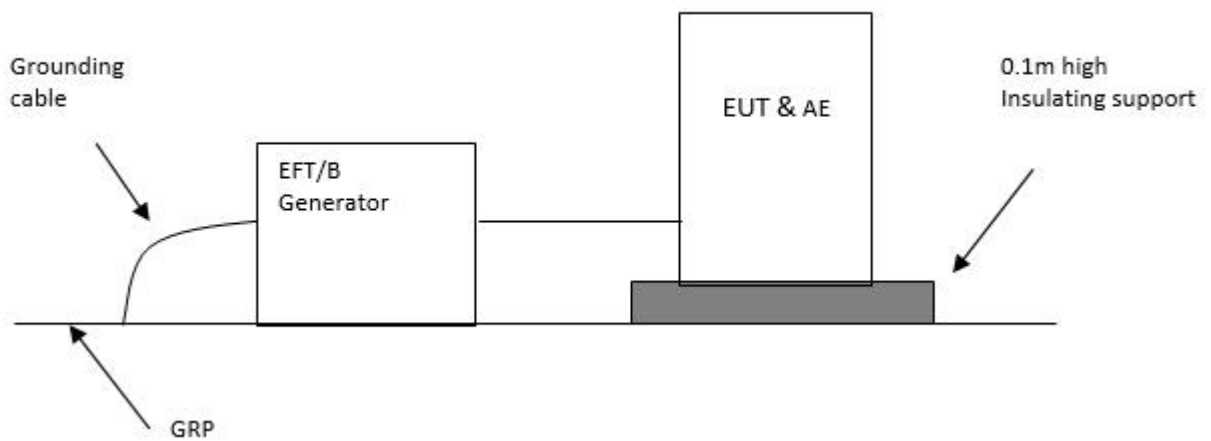

(for input a.c./d.c. power line)

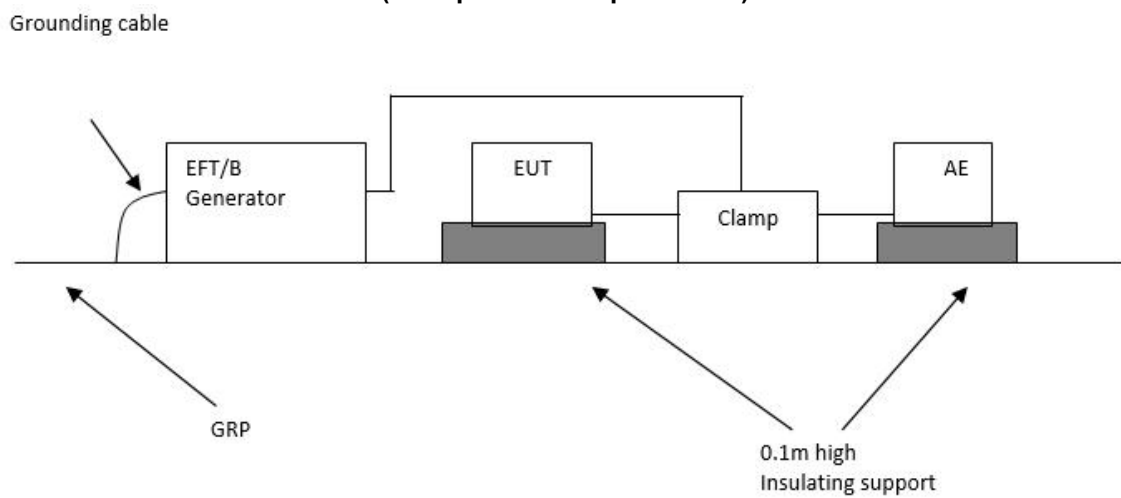

(for output a.c./d.c. power line or signal/control lines)

Test Procedures:

- 1) The EUT was placed on a ground reference plane (GRP) insulated by an insulating support 0.1m thick



and the GRP was placed on a 0.8m high wooden table for table-top equipment. For floor standing equipment, the EUT was placed on a 0.1m high wooden support above the GRP.

- 2) The GRP shall project beyond the EUT and the clamp by at least 0.1m on all sides. The distance between the EUT and any other of the metallic surface except the GRP was greater than 0.5m. All cables to the EUT was placed on the insulation support 0.1m above GRP. A cable not subject to EFT was routed as far as possible from cable under test to minimize the coupling between the cables.
- 3) The length of signal and power cable between the EUT and EFT generator was 0.5m. If the cable is a non-detachable supply cable more than 0.5m, the excess length of this cable shall be folded to avoid a flat coil and situated at a distance of 0.1m above the GRP.
- 4) The EUT was conducted the below specified test voltages for line and neutral or line, neutral and earth simultaneously (for Wired network, single, control and DC port line with capacitive coupling clamp), 120 seconds duration. If the equipment contains identical ports, only one was tested; multicomputer cables, such as a 50-pair Wired network cable, were tested as a single cable. Cables did not be split or divided into groups of conductors for this test; interface ports, which were intended by the manufacturer to be connected to data cables not longer than 3 m, did not be tested.


Equipment Used: Refer to section 3 for details.


Test Result: See below table.

| Test Ports | Test Level | Result | |
|--|----------------------------|---|--|
| | | (Pursuant to EN IEC 55014-2:2021 Criterion B) | |
| AC mains power ports | ± 0.5 kV, ± 1.0 kV | <input checked="" type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) |
| DC mains power ports | ± 0.5 kV | <input type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) |
| Signal lines and control lines | ± 0.5 kV | <input type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) |
| Observation: <input checked="" type="checkbox"/> No observable change. <input type="checkbox"/> During the experiment, the following phenomena occurred: <hr/> | | | |
| Conclusion: The EUT met the requirements of the standard. | | | |

6.3.4 Injected currents

| | |
|----------------------------|---|
| Test Requirement: | EN IEC 55014-2:2021 Clause 5.3, 5.4 |
| Test Method: | The test method shall be in accordance with EN 61000-4-6 |
| Criterion Required: | performance criteria A |
| Test Level: | for signal lines and control lines: 1 V (r.m.s) Input and output d.c. power ports: 1 V (r.m.s) Input and output a.c. power ports: 3 V (r.m.s) |
| Test Frequency: | 0.15 MHz to 80 MHz or 0.15 MHz to 230 MHz |
| Modulation: | 80%, 1kHz Amplitude Modulation |
| Step Size: | 1% increment |
| Dwell Time: | 1s |
| Test Setup: | |

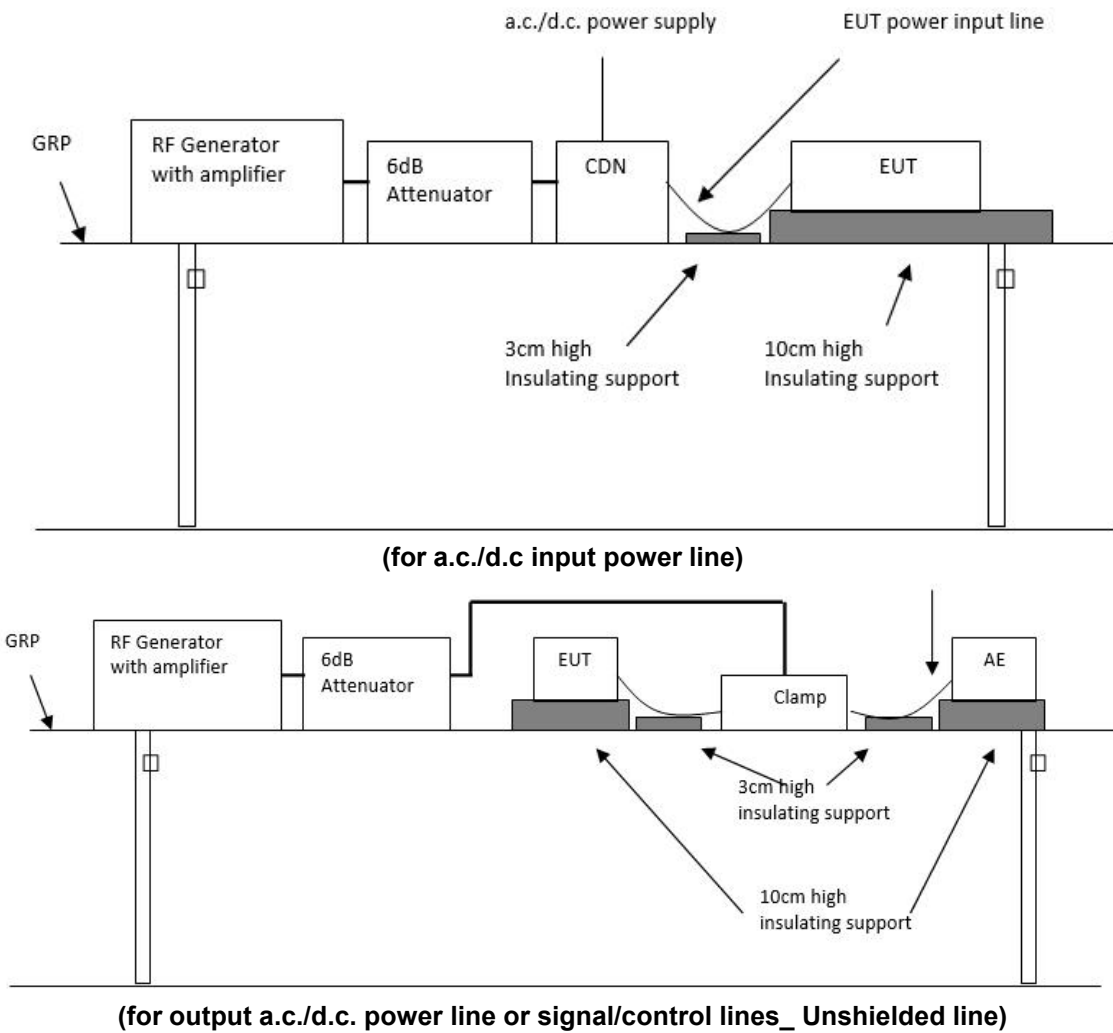

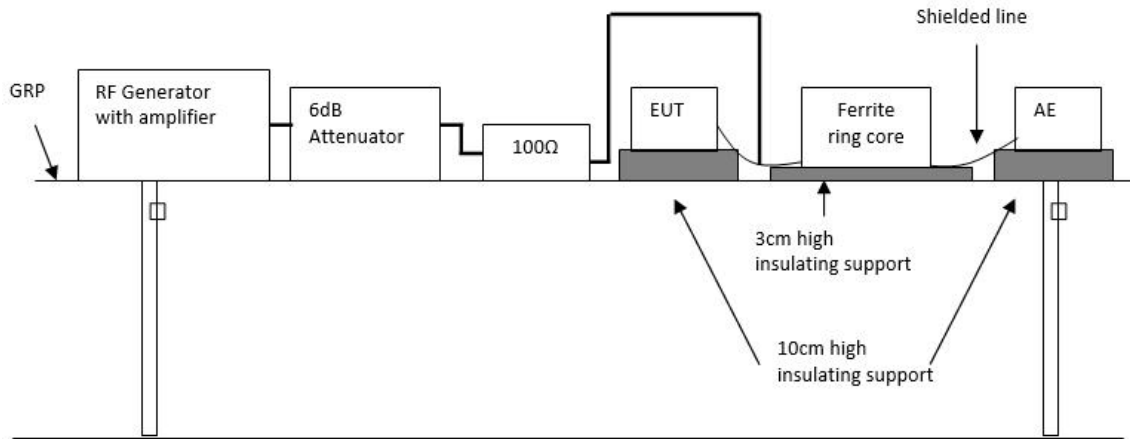

(for output a.c./d.c. power line or signal/control lines_ Shielded line)

Test Procedures:

- 1) The Product and support units were located at a ground reference plane with the interposition of a 0.1 m thickness insulating support and the CDN was located on GRP directly.
- 2) The frequency range is swept from 150 kHz to 80MHz, with the signal 80% amplitude modulated with a 1 kHz sine wave. The rate of sweep did not exceed 1.5×10^{-3} decade/s. Where the frequency range is swept incrementally, the step size was 1% of fundamental.
- 1) The dwell time at each frequency shall be not less than the time necessary for the Product to be able to respond.

Equipment Used: Refer to section 3 for details.

Test Result: See below table.

For EUT test Electromagnetic field susceptibility

| Test Ports | Frequency | Test Level | Result (Pursuant to EN IEC 55014-2:2021 Criterion A) |
|----------------------|--------------------|------------|--|
| AC mains power ports | 0.15 MHz to 80 MHz | 3 V | A |


Observation:

- No observable change.
- During the experiment, the following phenomena occurred:

Conclusion: The EUT met the requirements of the standard.

6.3.5 Surges

| | |
|----------------------------|--|
| Test Requirement: | EN IEC 55014-2:2021 Clause 5.6 |
| Test Method: | The test method shall be in accordance with EN 61000-4-5 |
| Criterion Required: | performance criteria B |
| Wave Shape: | 1.2/50 (8/20) μ s |
| Test Level: | for AC mains power ports: 2kV line-to-earth with 12 Ω Impedance and 1 kV line-to-line with 2 Ω Impedance. |
| Polarity: | Positive & Negative |
| Interval: | 60s between each surge |
| No. of Surges: | 5 positive at 90°, 5 negative at 270° |
| Test Setup: | |

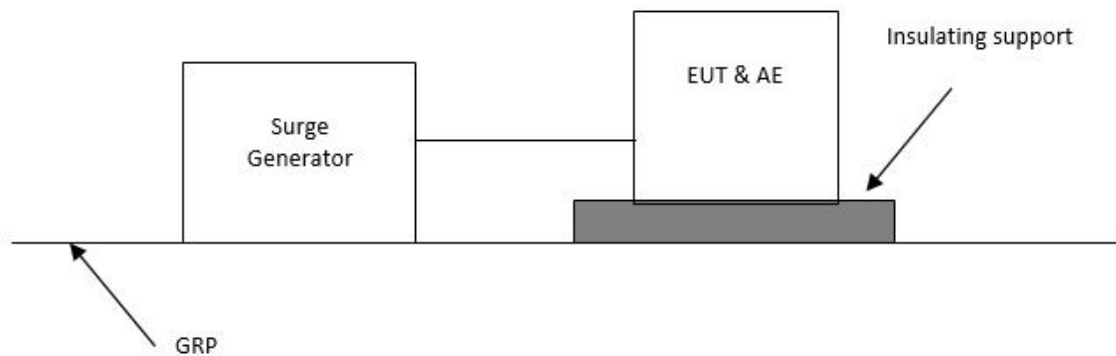

Test Procedures:

Test Procedure:

- 1) The EUT was placed on a ground reference plane (GRP) insulated by an insulating support 0.1 m thick and the GRP was placed on a 0.8m high wooden table for table-top equipment. For floor standing equipment, the EUT was placed on a 0.1m high wooden support above the GRP.
- 2) The 1.2/50 μ s surge was to be applied to the EUT power supply terminals via the capacitive coupling network. Decoupling networks were required in order to avoid possible adverse effects on equipment not under test that may be powered by the same lines and to provide sufficient decoupling impedance to the surge wave so that the specified wave may be applied on the lines under test.
- 3) The power cord between the EUT and the coupling/decoupling network was not exceed 2 m in length. The interconnection line between the EUT and the coupling/decoupling network shall not exceed 2 m in length.
- 4) The EUT was conducted 0.5 kV and 1 kV test voltage for line to line and line to neutral and conducted 0.5 kV, 1 kV and 2 kV test voltage for line to earth and neutral to earth, five positive pulses and five negative pulses each at 90°, 270° for a.c. power ports and five positive pulses and five negative surge pulses for d.c. power ports, The test levels were applied on the EUT with a 2 Ω generator source impedance for power supply terminals and 12 Ω output impedance for interconnection lines. The tests were done at repetition rate one per minute.

Equipment Used: Refer to section 3 for details.



Test Result: See below table.

| For AC mains power port | | | | |
|---|--------------|---|--|---|
| Test Ports | Level | Result (Pursuant to EN IEC 55014-2:2021 Criterion B) | | |
| | | Between Phase And Neutral | ± 1.0 kV | <input checked="" type="checkbox"/> A |
| Between Phase And Earth | ± 2.0 kV | <input type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input checked="" type="checkbox"/> N/A |
| Between Phase And Earth | ± 2.0 kV | <input type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input checked="" type="checkbox"/> N/A |
| Remark: N/A: Not applicable | | | | |
| Observation: <input checked="" type="checkbox"/> No observable change. <input type="checkbox"/> During the experiment, the following phenomena occurred: | | | | |
| Conclusion: The EUT met the requirements of the standard. | | | | |

6.3.6 Voltage dips


Test Requirement: EN IEC 55014-2:2021 Clause 5.7
Test Method: The test method shall be in accordance with EN 61000-4-11
Criterion Required: performance criteria C
Test Port : AC mains power port
Test Level:

| Test level % UT | Voltage dip and short interruptions % UT | Duration (in period) | |
|--------------------|---|-------------------------|-----------|
| | | 50Hz | 60Hz |
| 0 | 100 | 0.5 cycle | 0.5 cycle |
| 40 | 60 | 10 cycles | 12 cycles |
| 70 | 30 | 25 cycles | 30 cycles |

Notes:

1. —*|| for 0.5 period, the test shall be made in positive and negative polarity, i.e. starting at 0° and 80°, respectively.
2. -**|| means -x|| is an open duration. This duration can be given in the product specification. Utilities in Europe have measured dips and short interruptions of duration between ½ a period and 3000 periods, but duration less than 50 periods are most common.
3. If the EUT is tested for voltage dips of 100%, it is generally unnecessary to test for other levels for the same durations. However, for some cases (safeguard systems or electro-mechanical devices) it is not true. The product specification or product committee shall give an indication of the applicability of this note.
4. The gray rows are selected test level.

Test Setup:

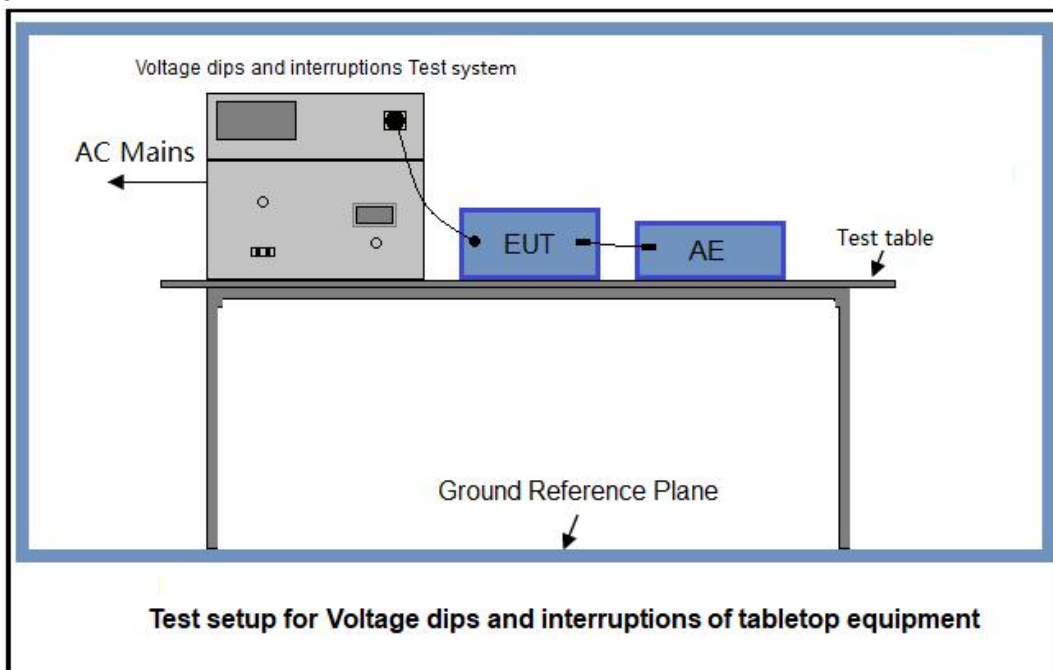

Test Procedures:

- 1) The EUT was placed on a ground reference plane (GRP) insulated by an insulating support 0.1 m thick and the GRP was placed on a 0.8m high wooden table for table-top equipment. For floor standing equipment, the EUT was placed on a 0.1m high wooden support above the GRP.
- 2) The test was performed with the EUT connected to the test generator with the shortest power supply cable as specified by the EUT manufacturer.
- 3) The EUT was tested for each selected combination of test level and duration with a sequence of three dips /interruptions with intervals of 10 s minimum. Each representative mode of operation was tested.
- 4) For EUT with more than one power cord, each power cord was tested individually.

Equipment Used: Refer to section 3 for details.



Test Result: See below table.



| Test Condition | | Result (Pursuant to EN IEC 55014-2:2021 Criterion C) | | |
|-------------------|------------------------------|--|--|--|
| Test Level in %UT | Period | | | |
| 0 | 0.5 | <input checked="" type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input type="checkbox"/> C(see phenomena) |
| 40 | 10 for 50 Hz 12 for 60 Hz | <input type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input checked="" type="checkbox"/> C(see phenomena) |
| 70 | 25 for 50 Hz 30 for 60 Hz | <input type="checkbox"/> A | <input type="checkbox"/> B (see phenomena) | <input checked="" type="checkbox"/> C(see phenomena) |

Remark:
N/A: Not applicable


Observation:
 No observable change.
 During the experiment, the following phenomena occurred:
EUT unit turned off at 40%UT and 70% test level with 10 and 25cycles (at 50Hz) duration and restore the working state manually.

Conclusion: The EUT met the requirements of the standard.

APPENDIX 1 PHOTOGRAPHS OF TEST SETUP

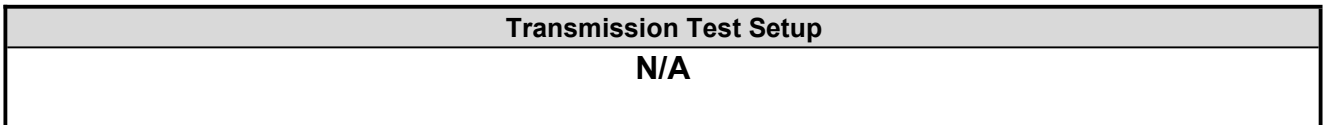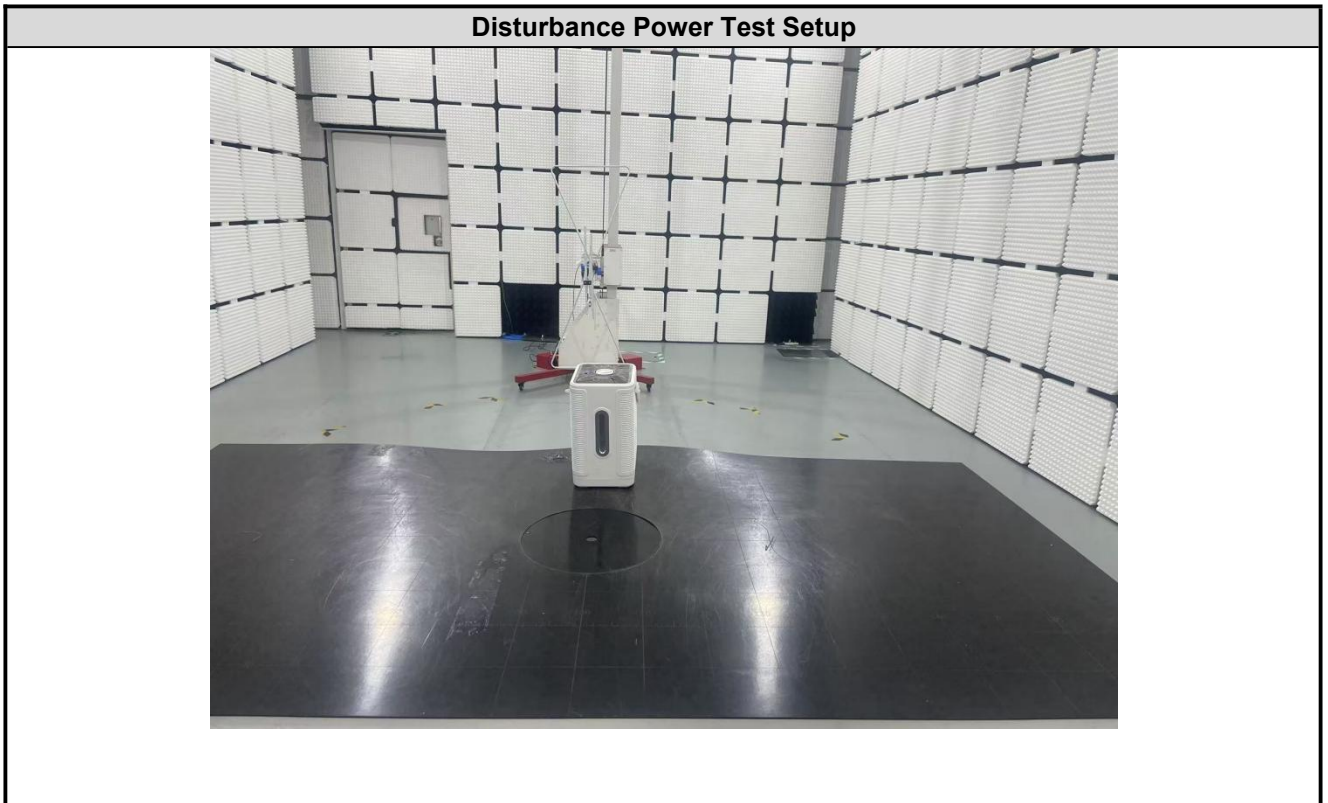

APPENDIX 2 PHOTOGRAPHS OF EUT CONSTRUCTIONAL DETAILSEUT EXTERNAL PHOTOS

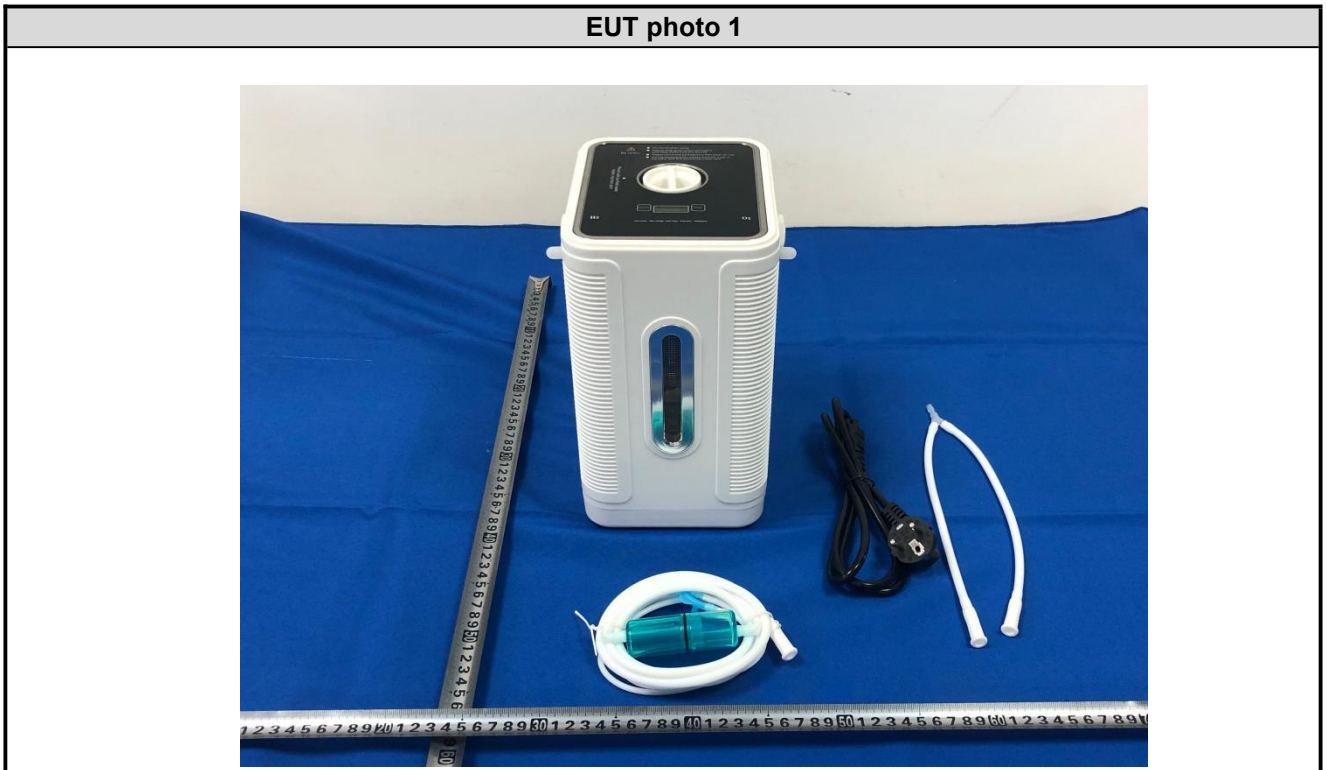


EUT photo 3




EUT photo 4



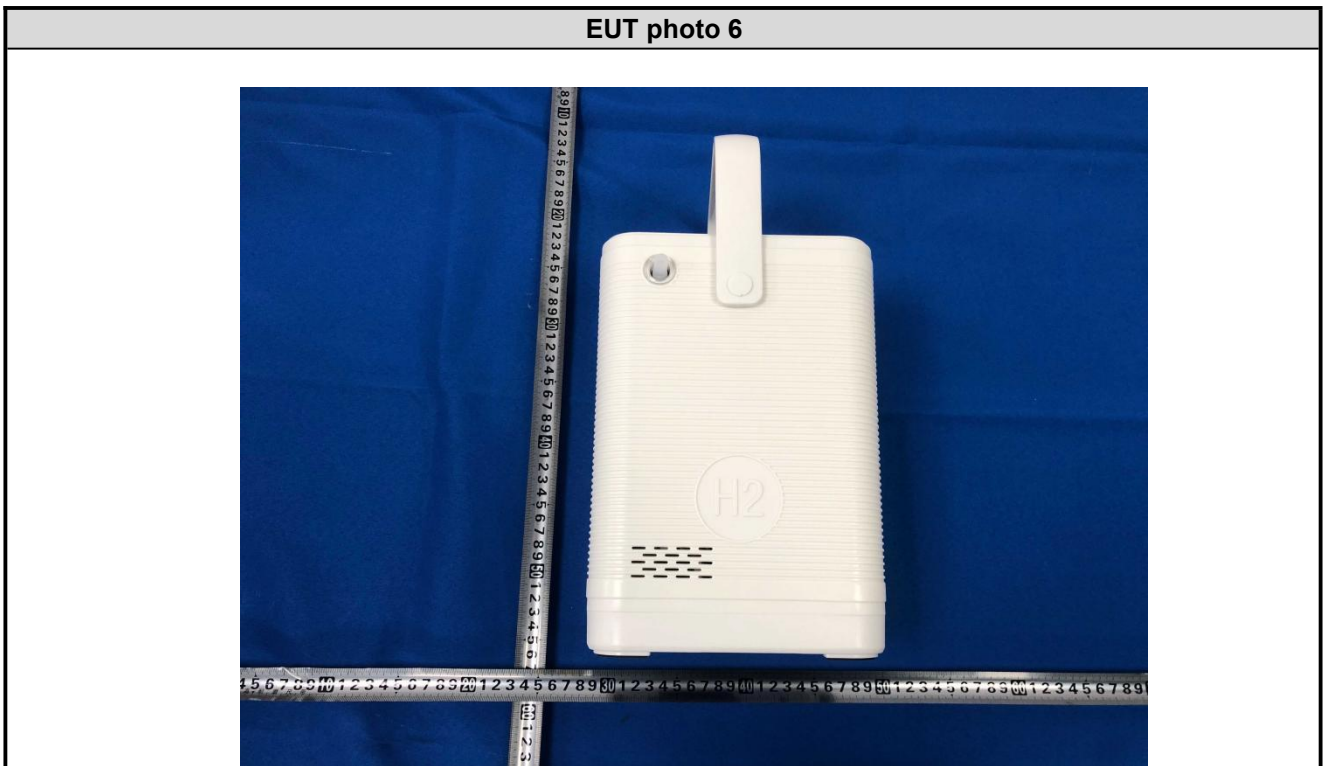


EUT INTERNAL PHOTOS


EUT photo 7

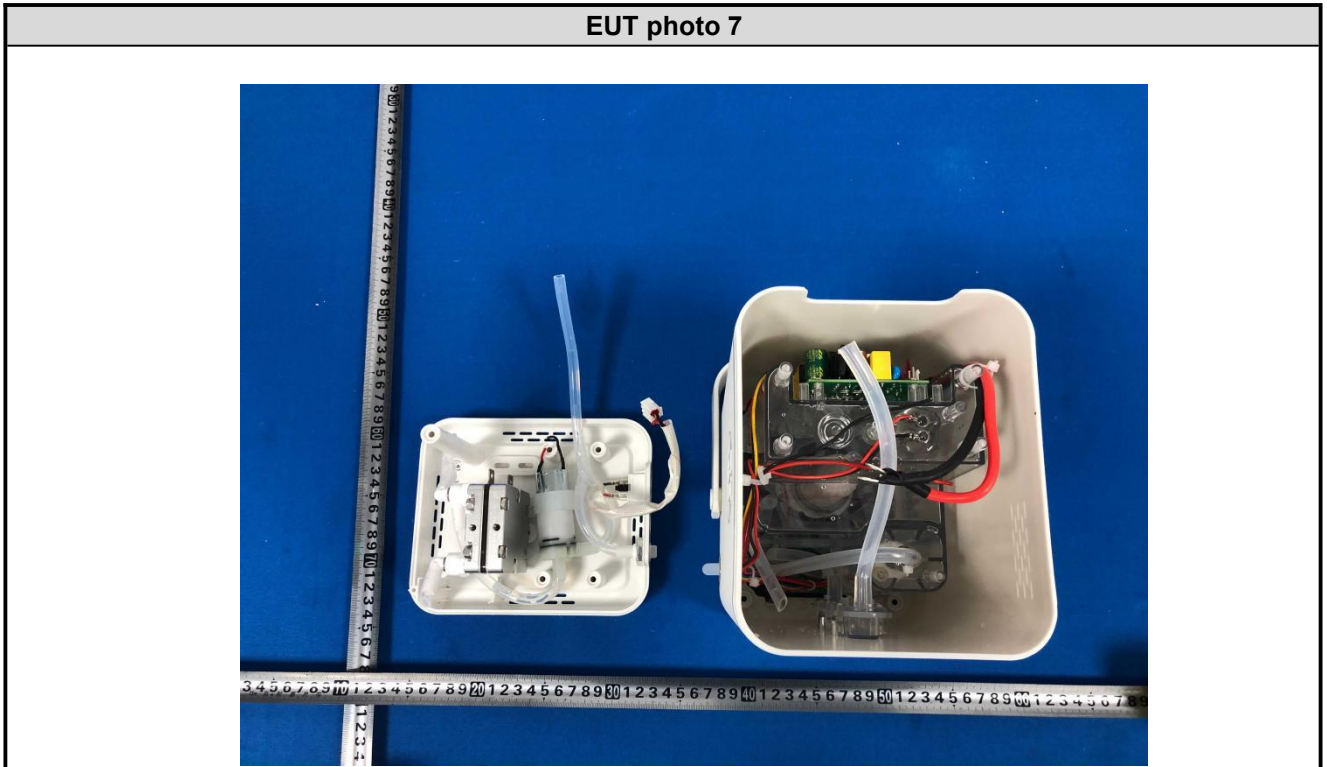


EUT photo 8

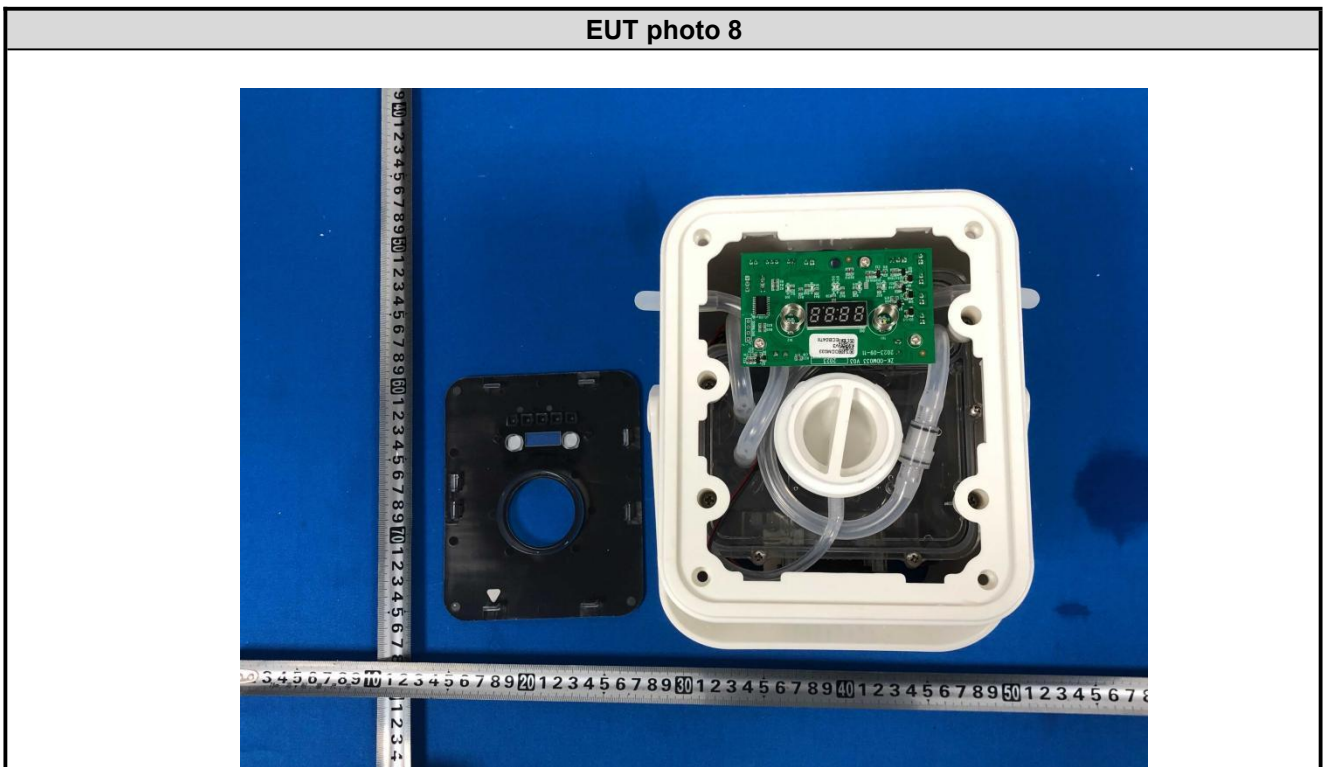


EUT photo 9

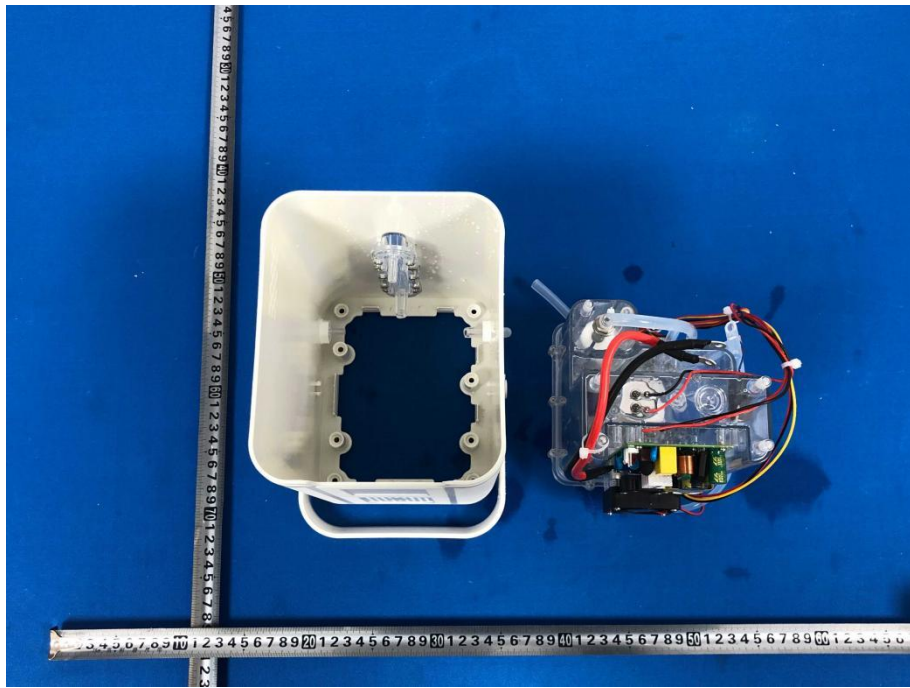


EUT photo 10

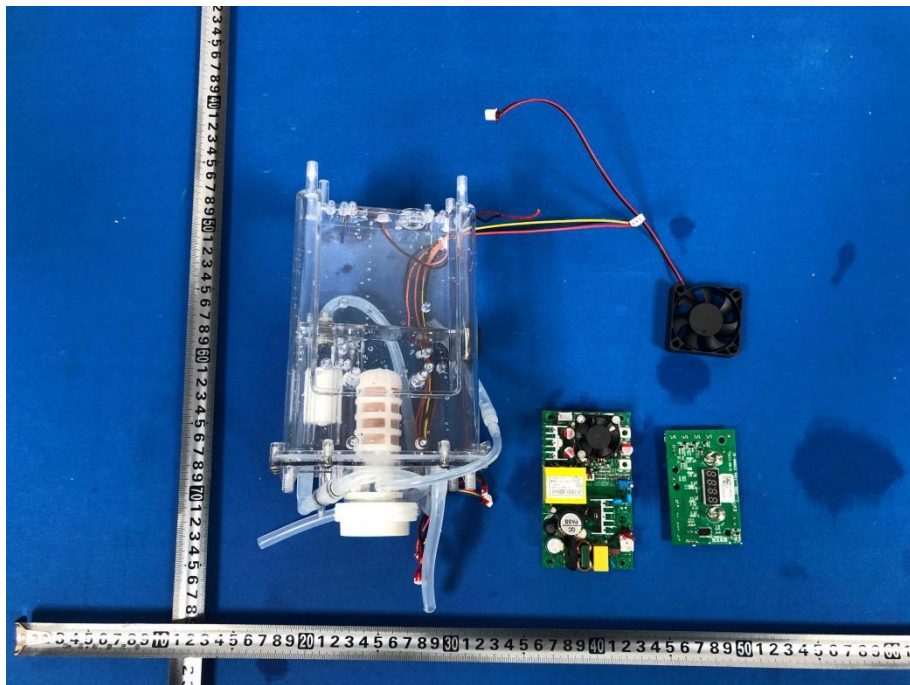


EUT photo 11

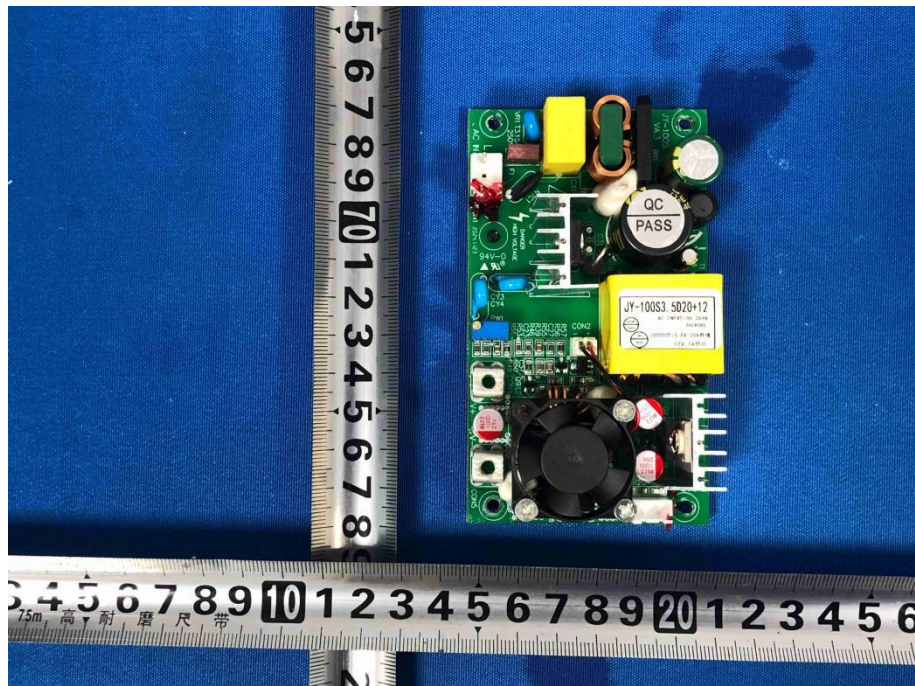


EUT photo 12

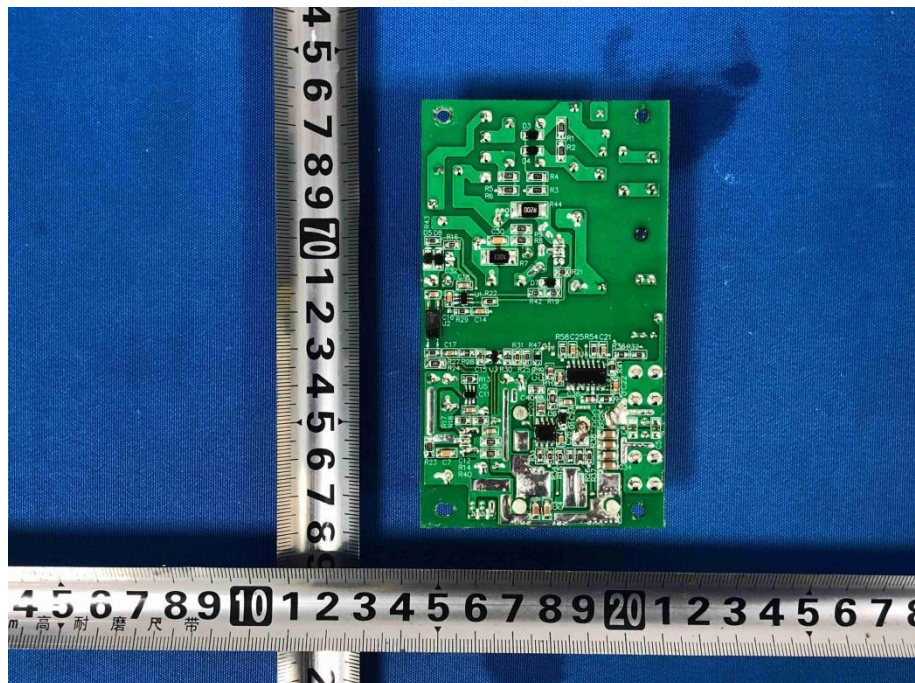

EUT photo 13

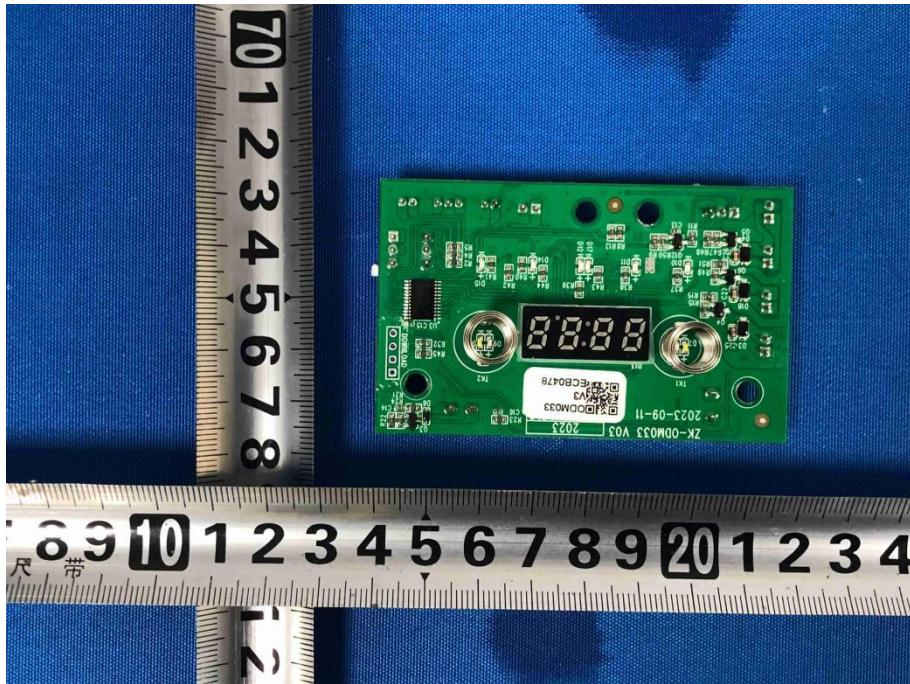

EUT photo 14

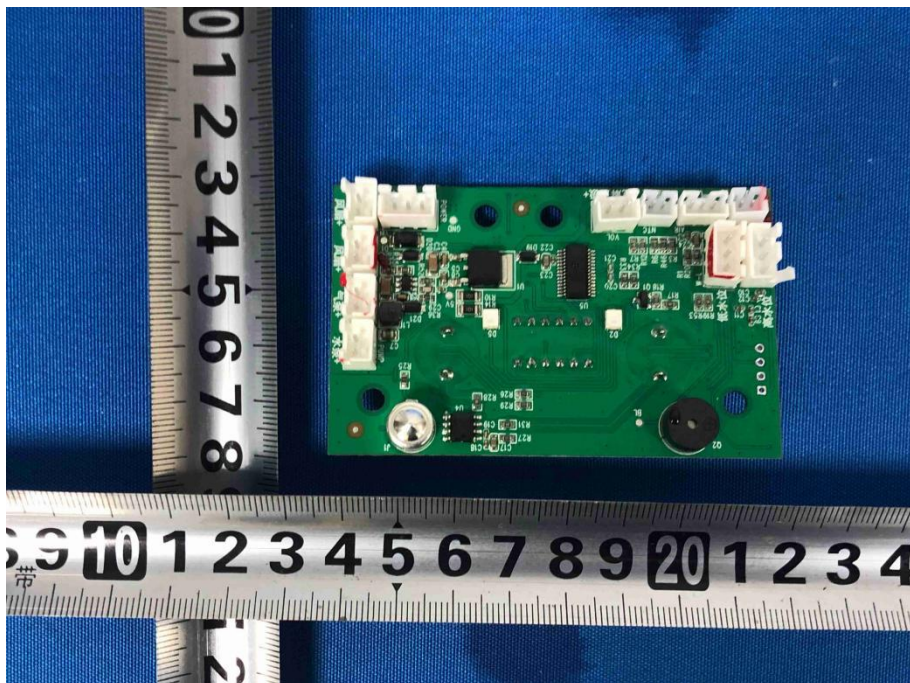



*** End of Report ***

The test report is effective only with both signature and specialized stamp. The result(s) shown in this report refer only to the sample(s) tested. Without written approval of UnionTrust, this report can't be reproduced except in full.
